

1/36

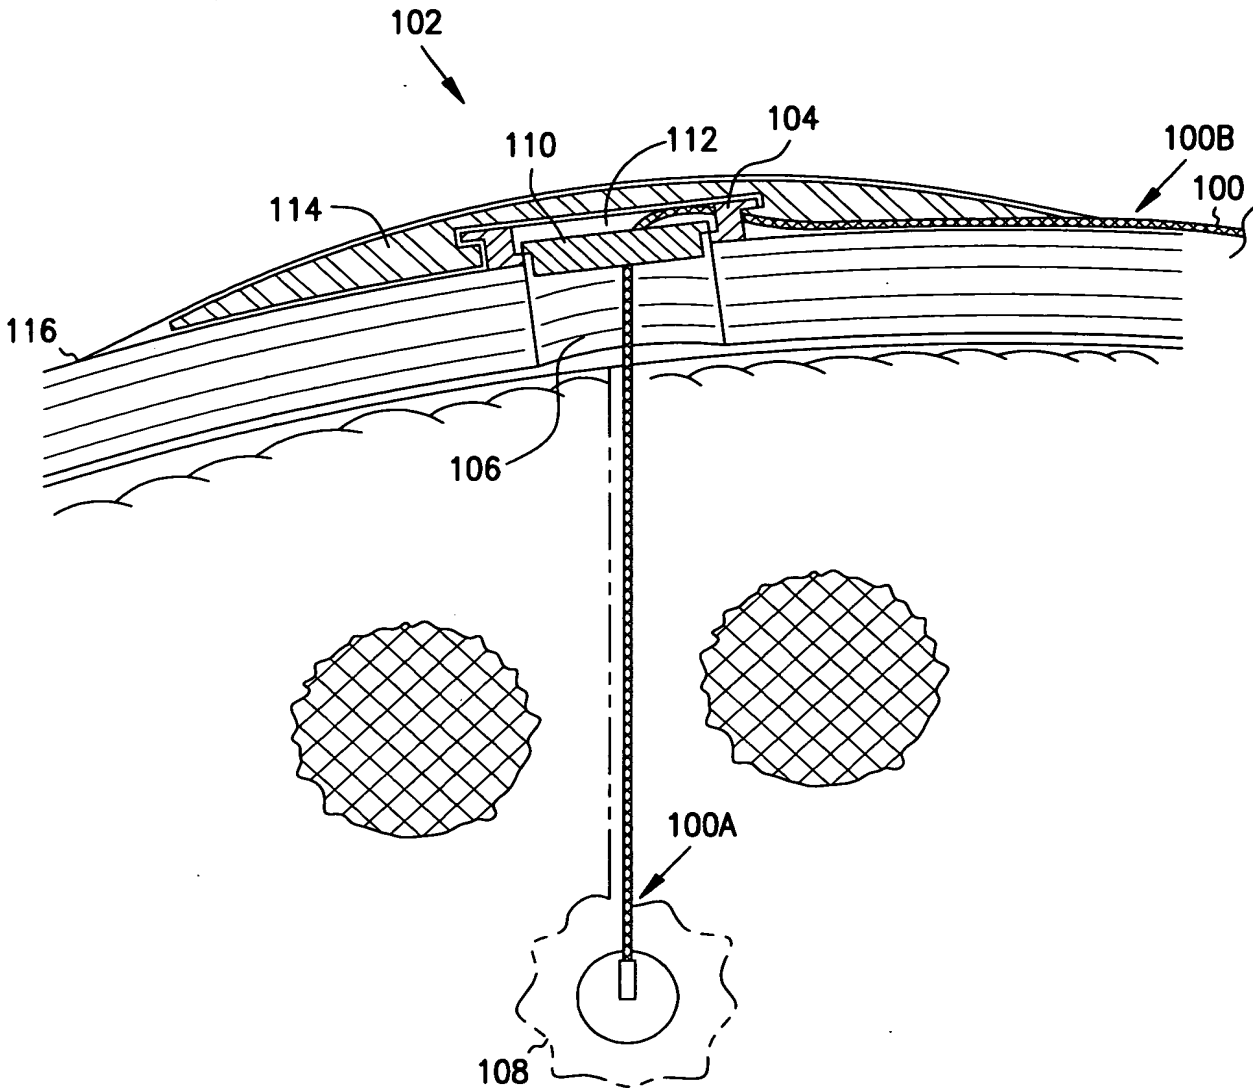


FIG. 1

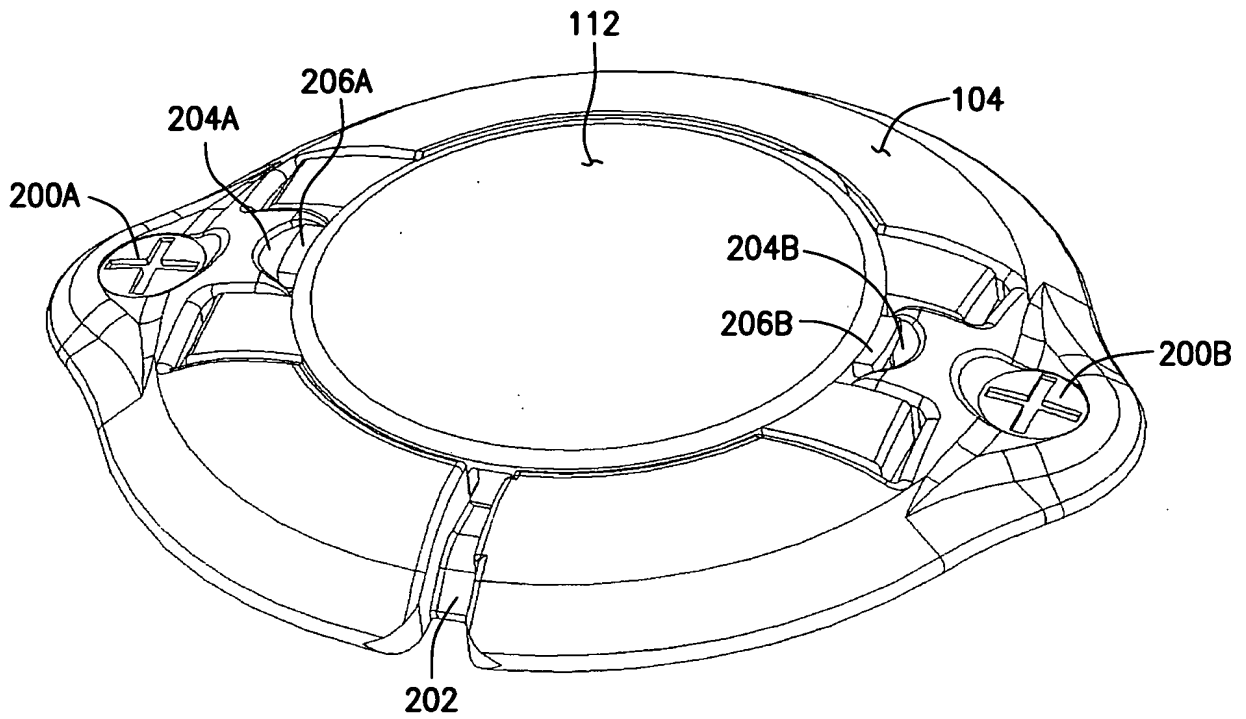


FIG. 2

3/36

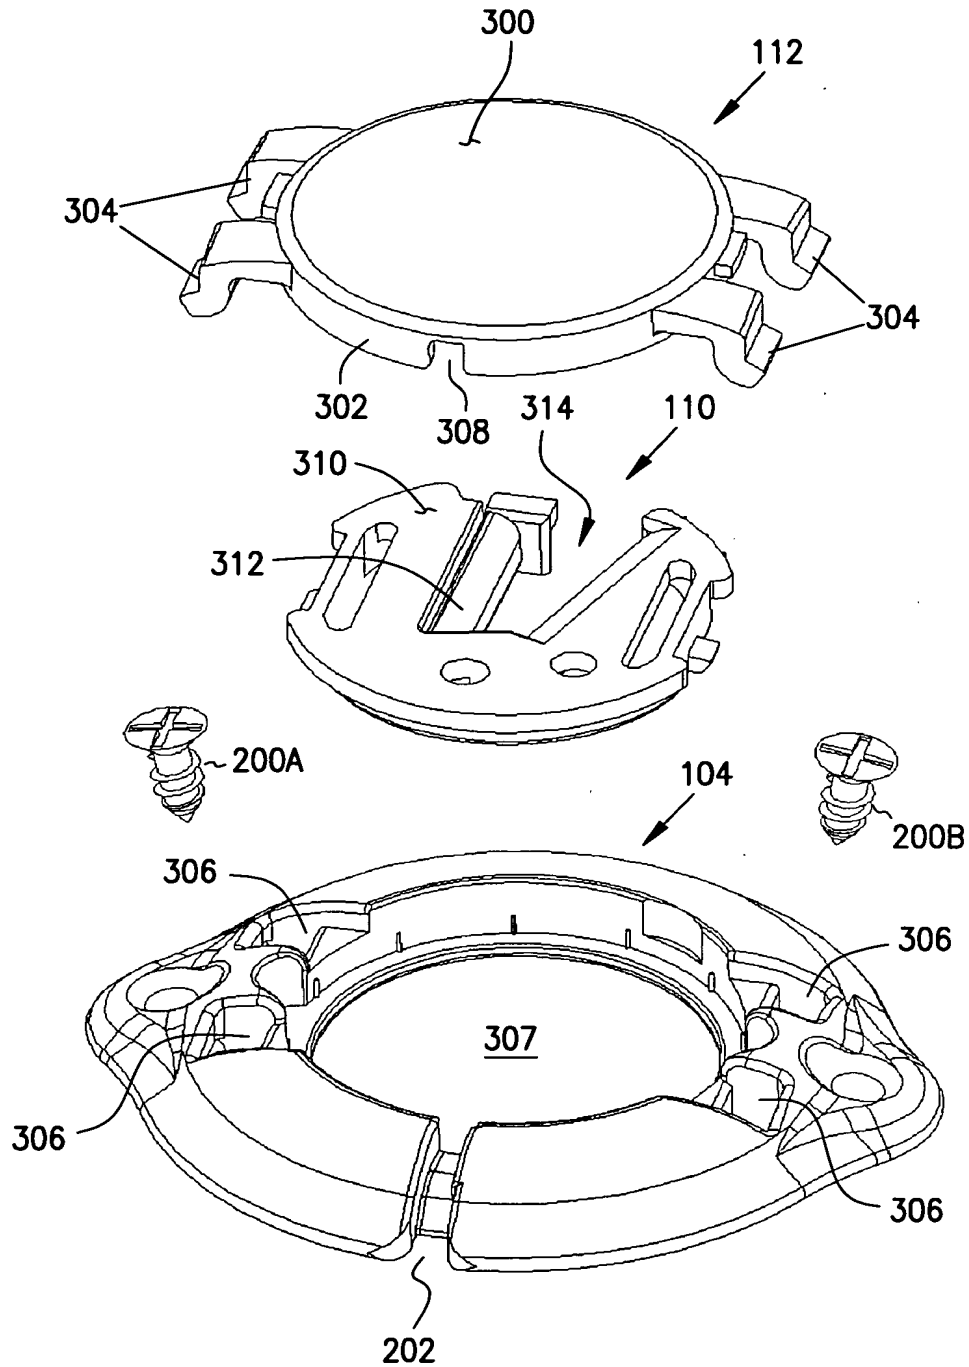


FIG. 3

09/828,451-0000

4/36

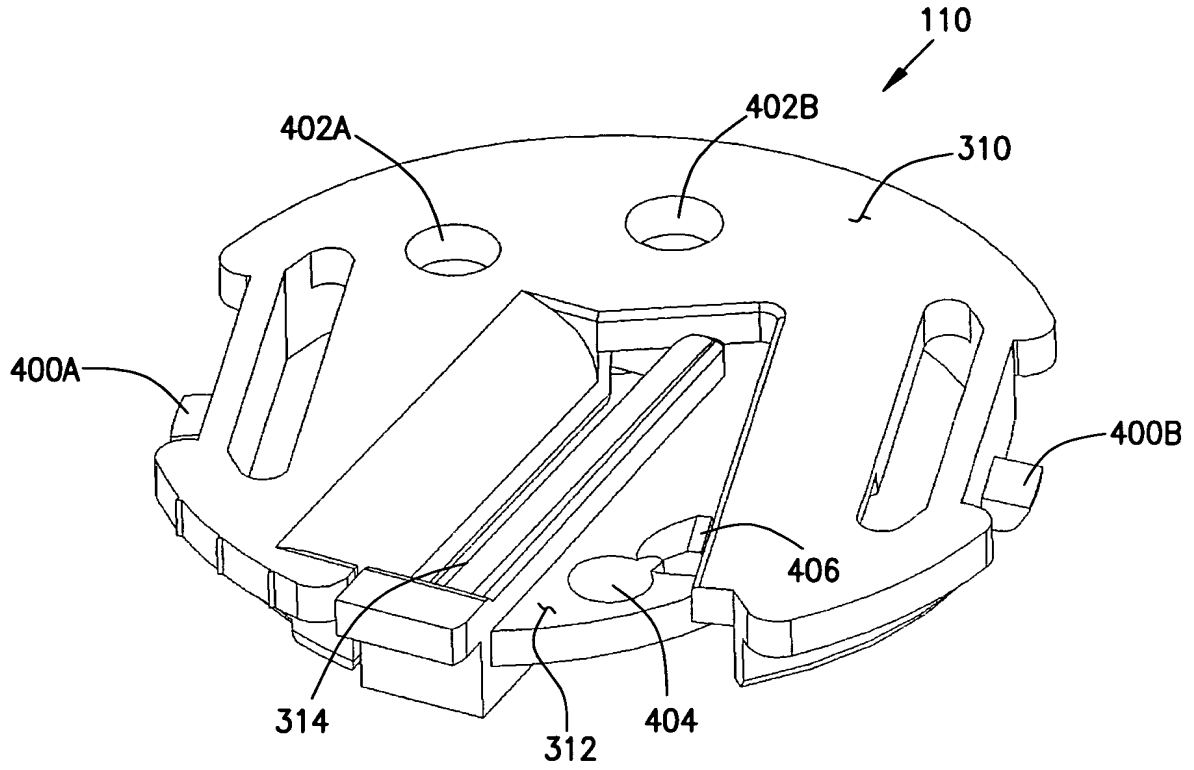


FIG. 4

09/828,451 03/2001

5/36

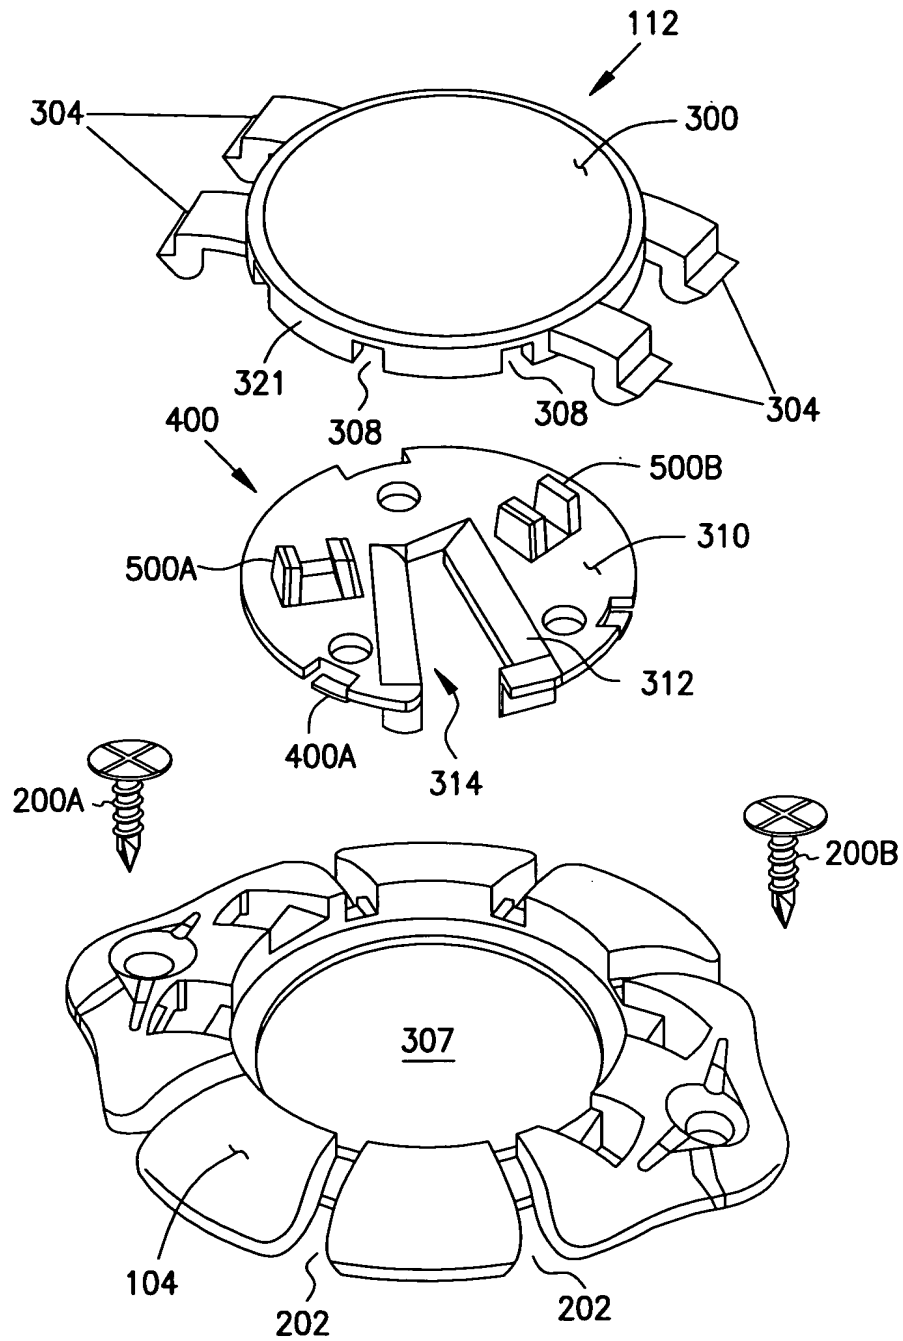


FIG. 5

6/36

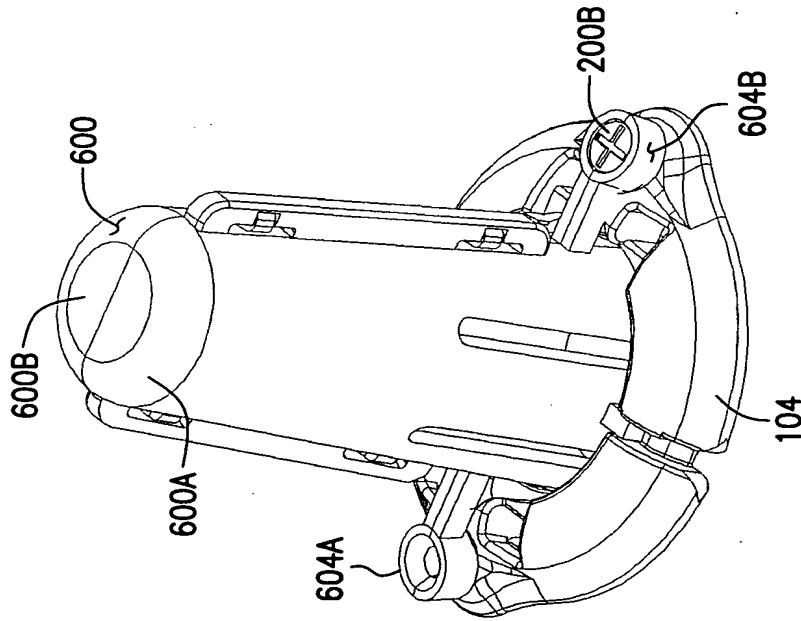
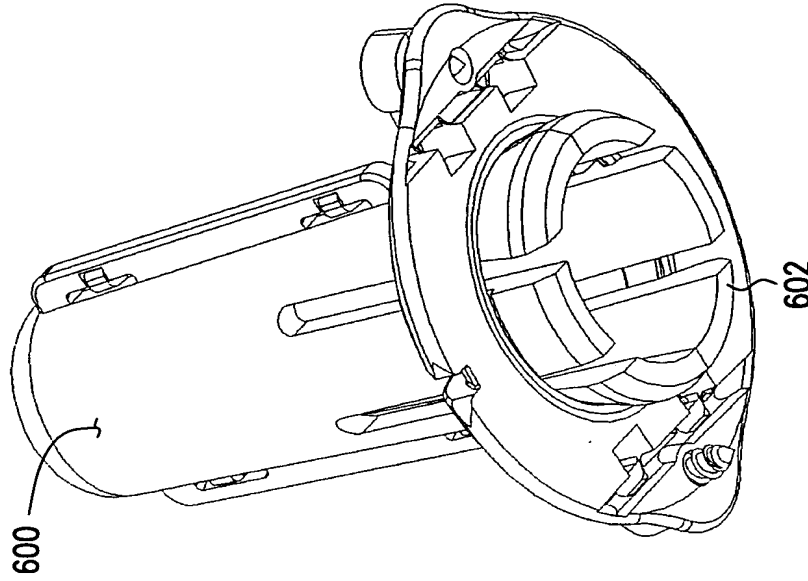


FIG. 6A

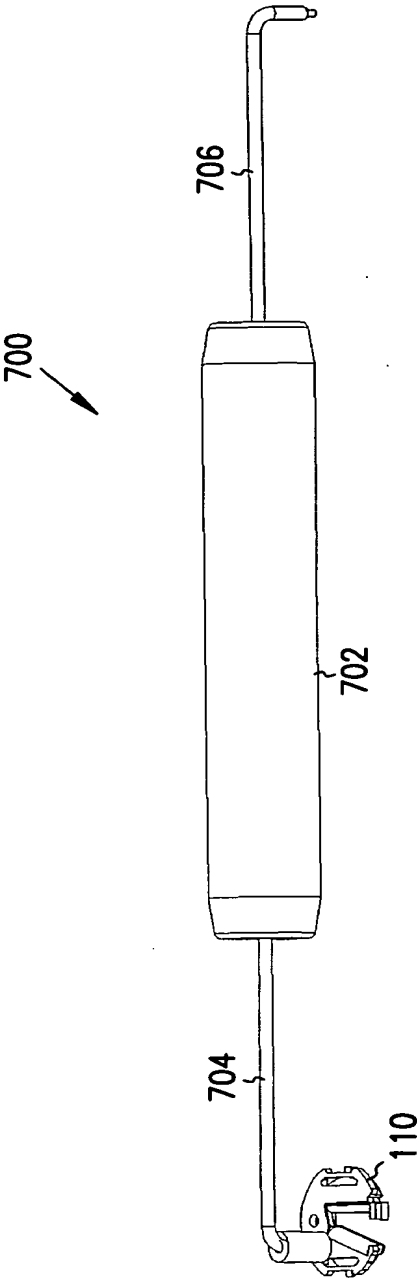


FIG. 7

8/36

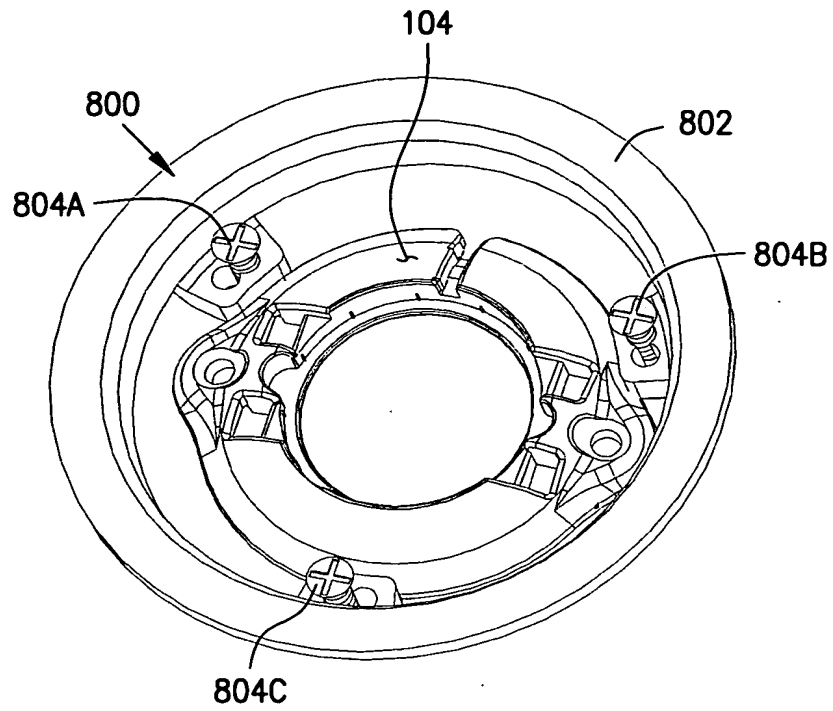


FIG. 8

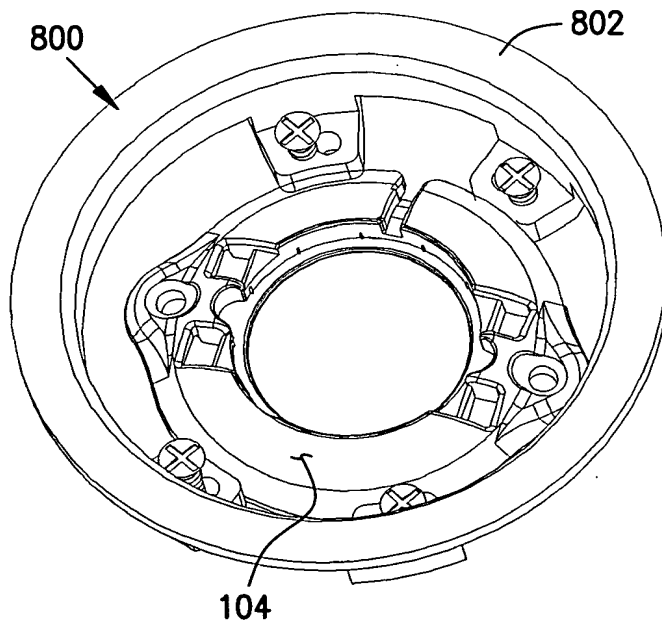


FIG. 9

09/828,451 100280 1542360



9/36


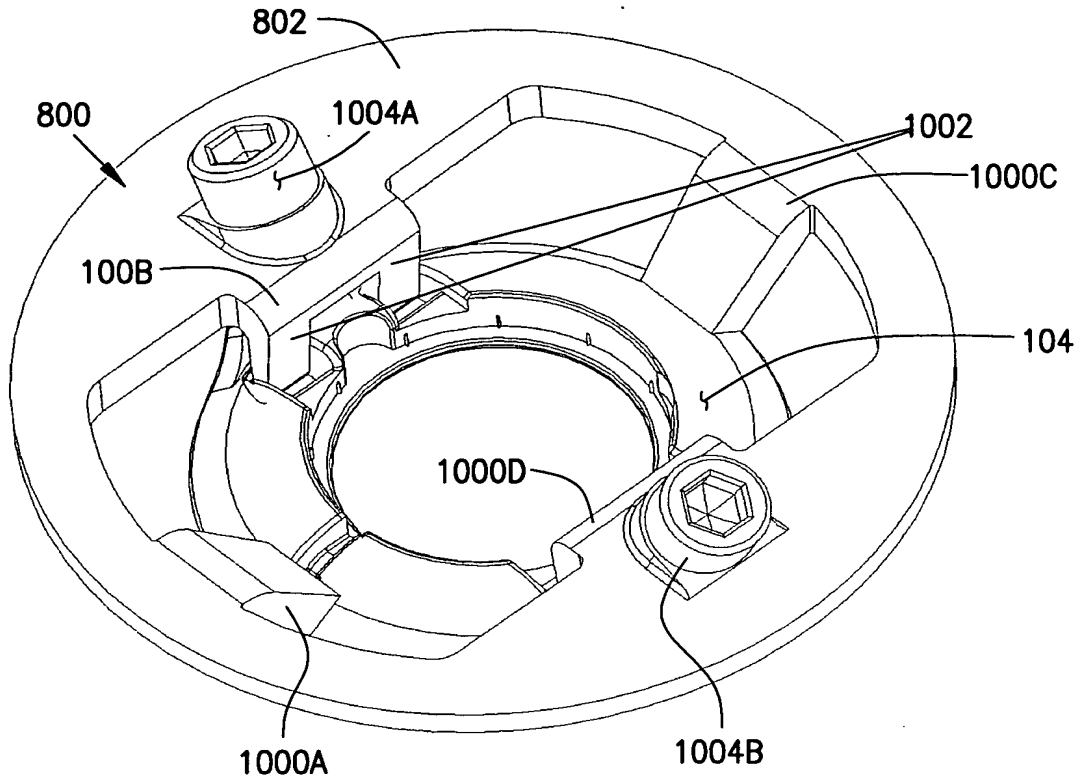


FIG. 10

09828451.082860

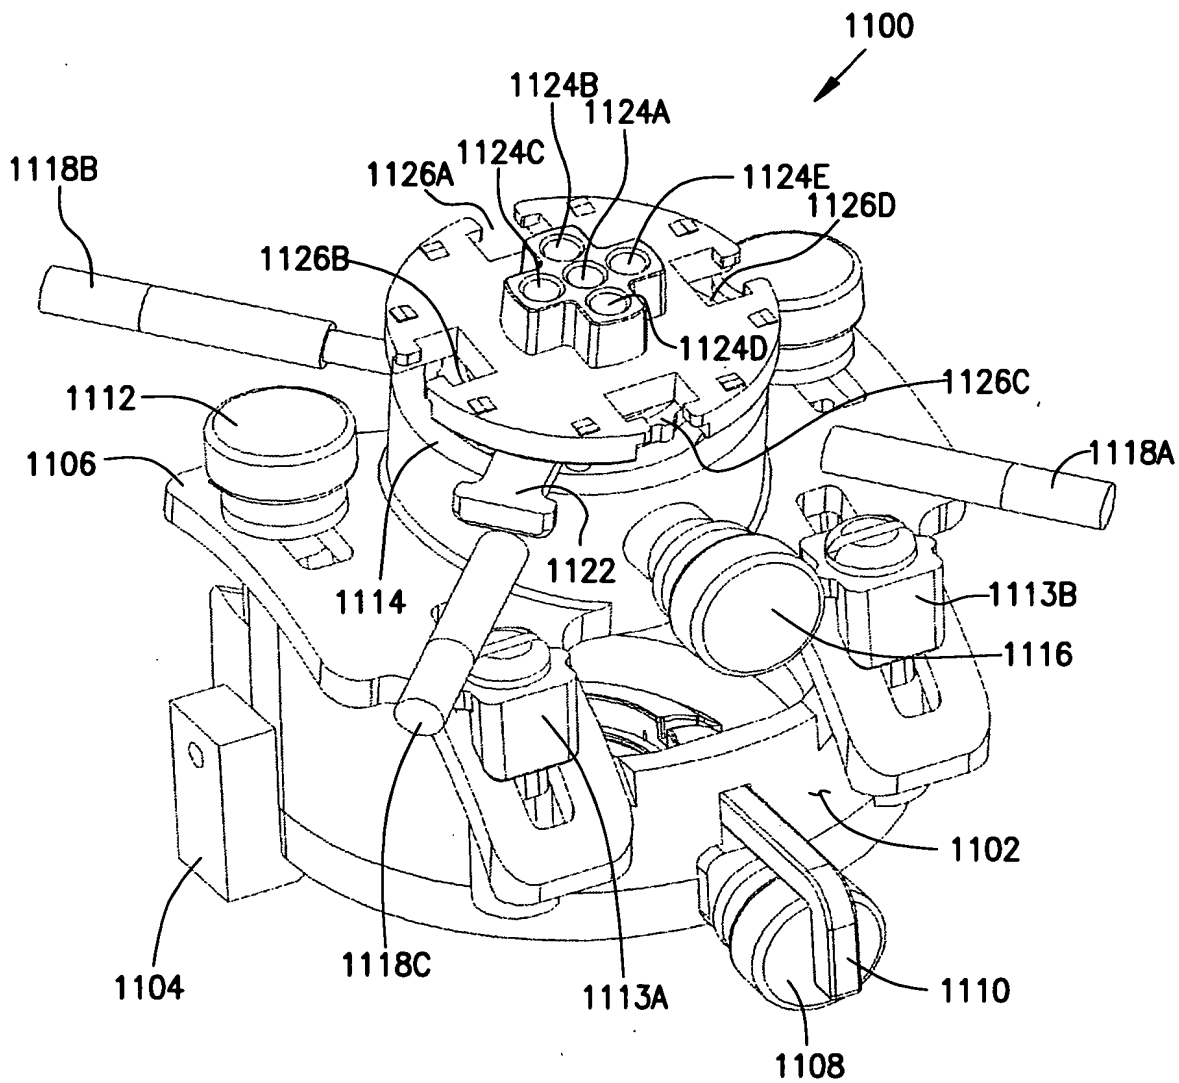

11/36

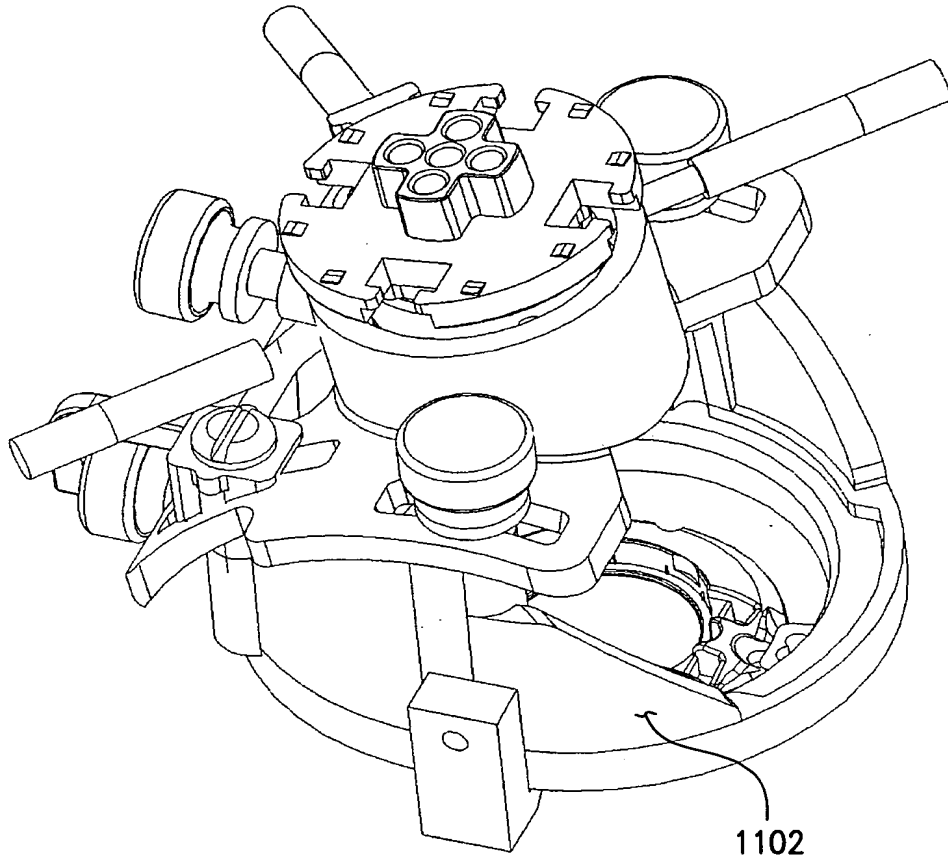


FIG. 12

12/36

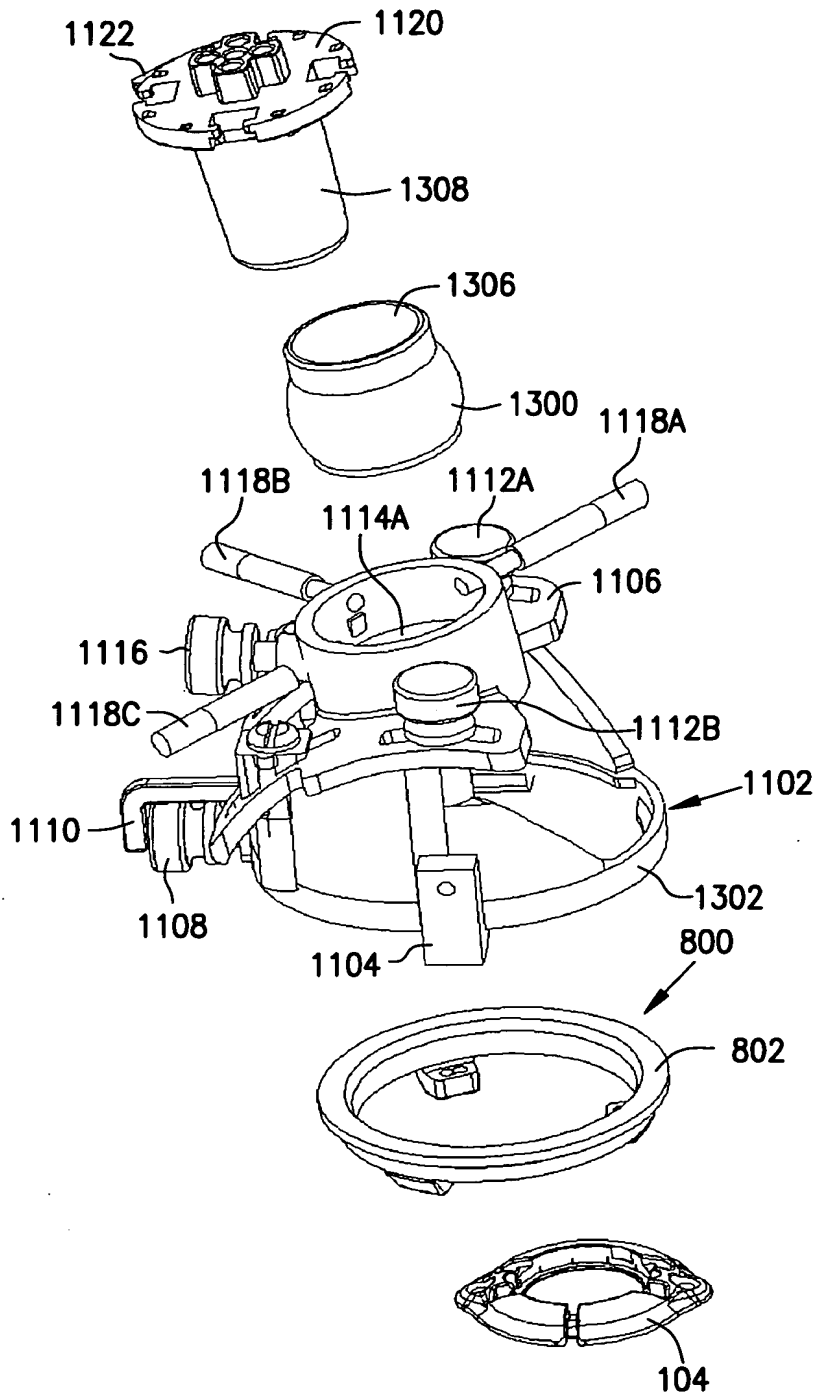


FIG. 13

09/828,451

13/36

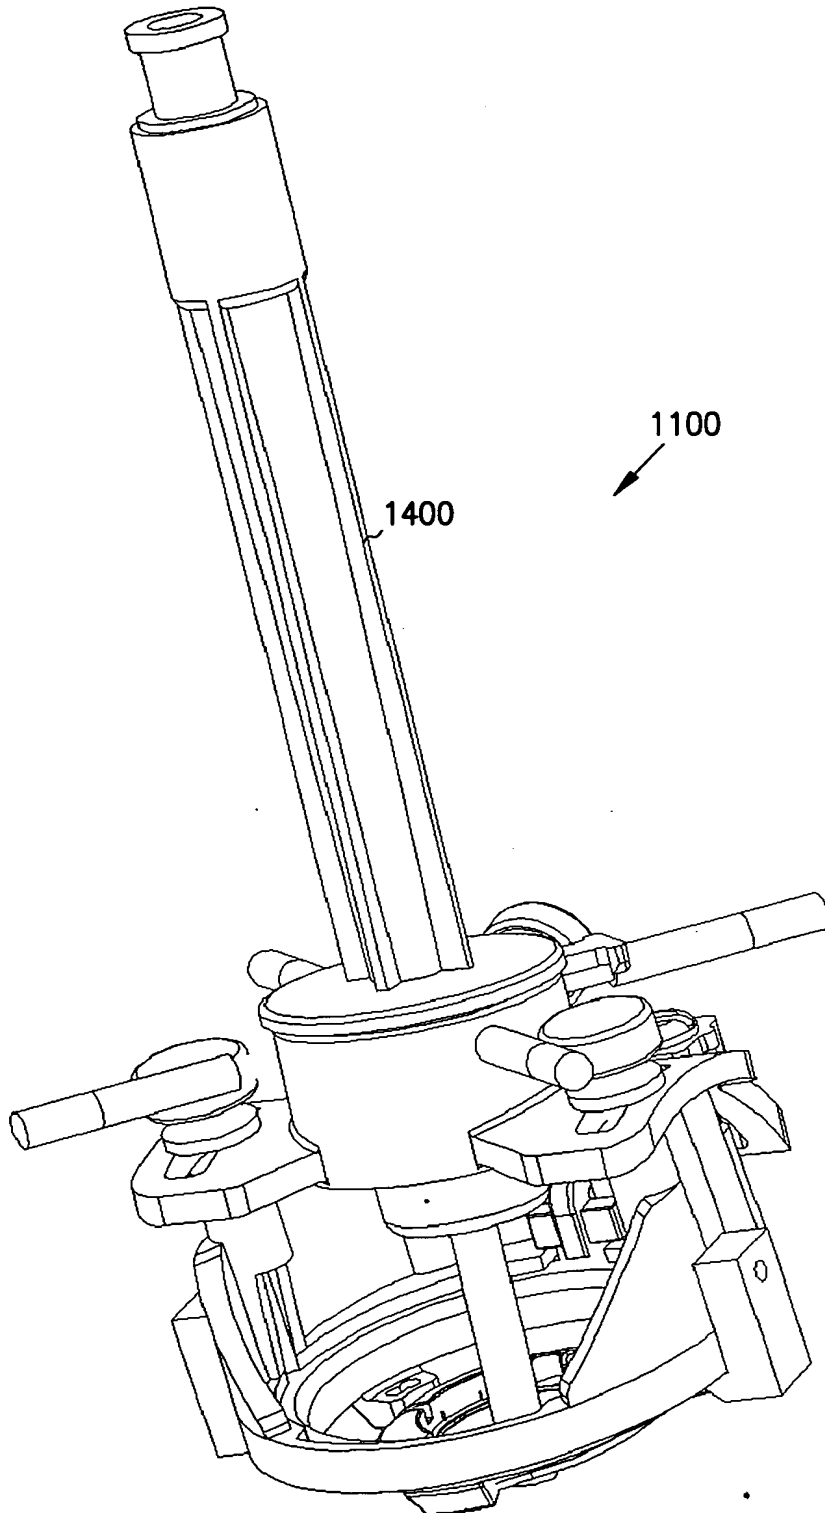


FIG. 14

09/828,451-082001

14/36

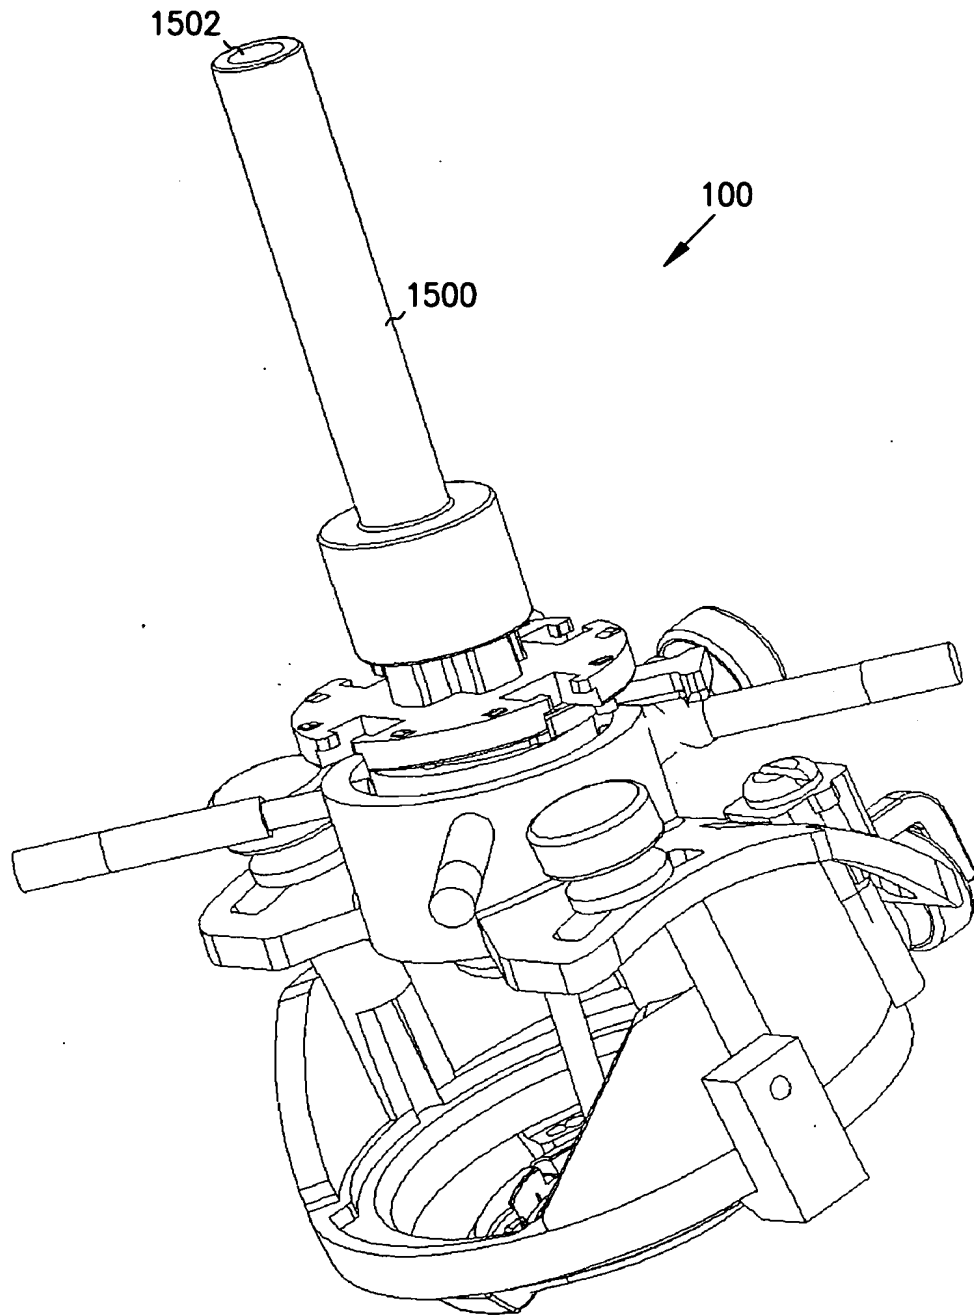


FIG. 15

09828451.082001

15/36

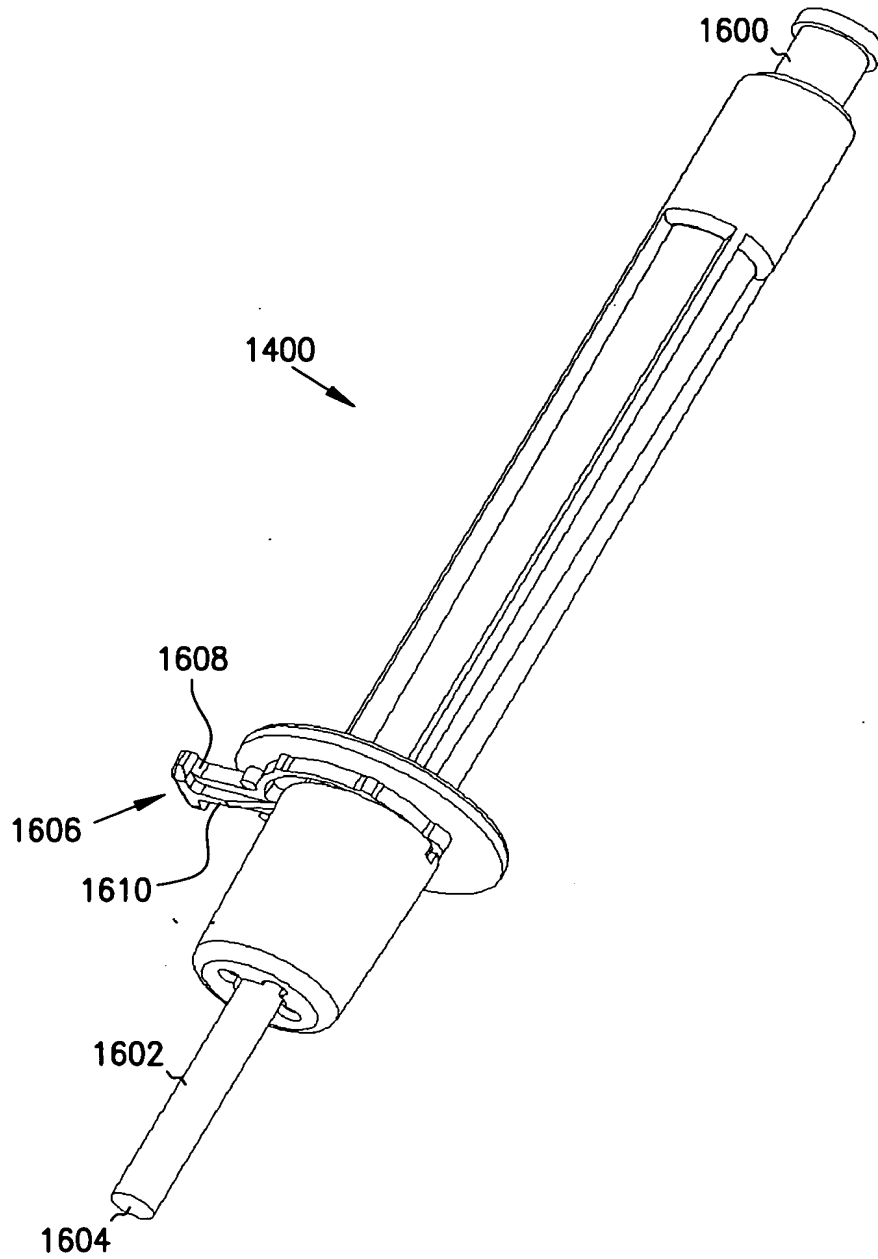


FIG. 16

09/828,451 0828001

16/36

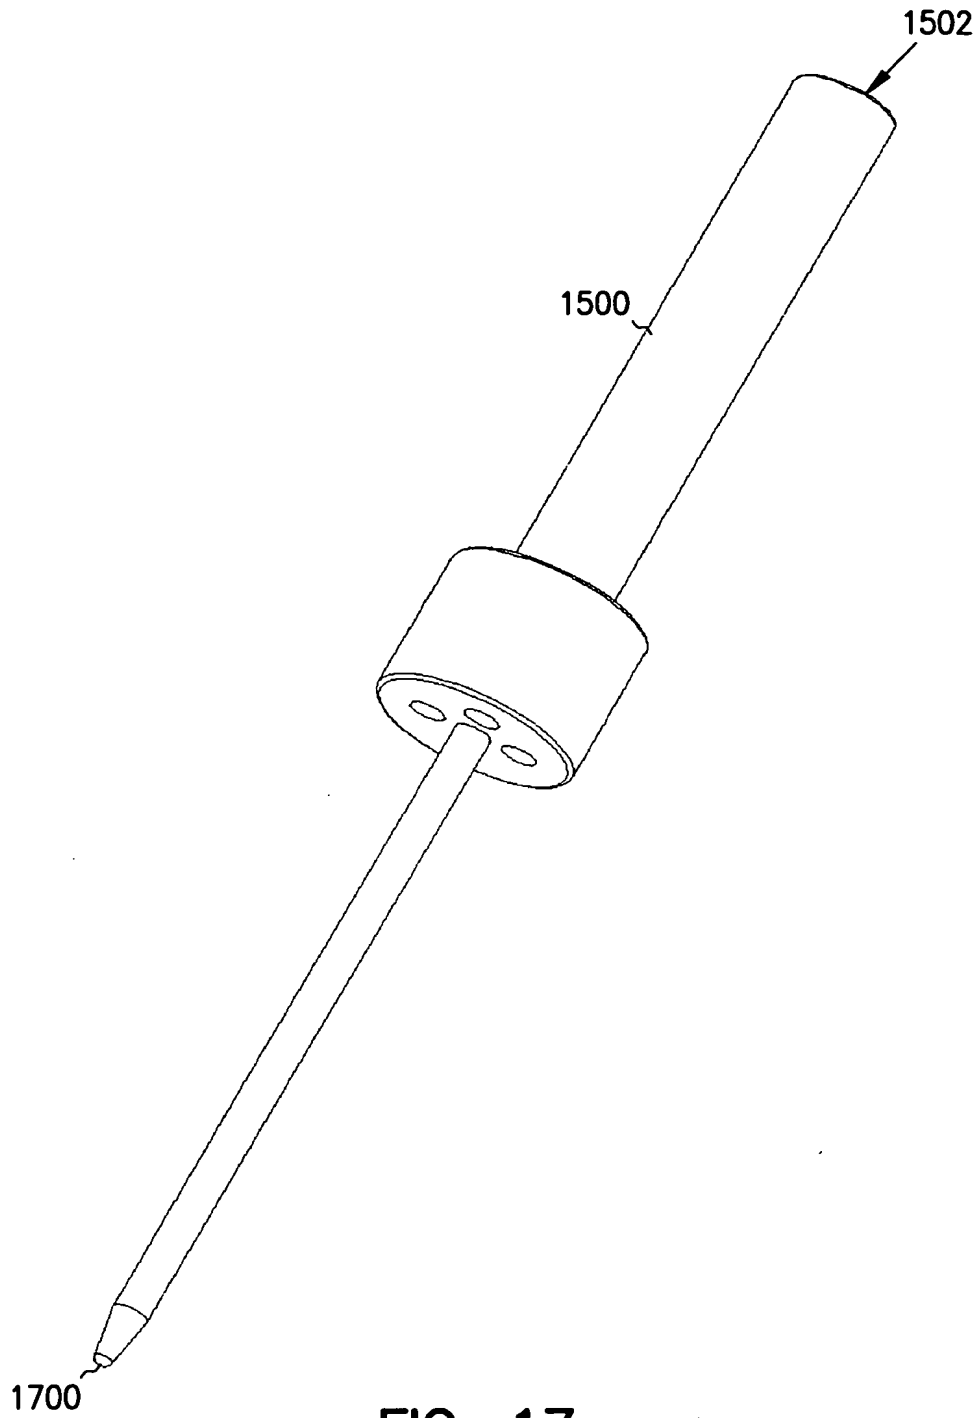


FIG. 17

09/828,451 F5432350



17/36

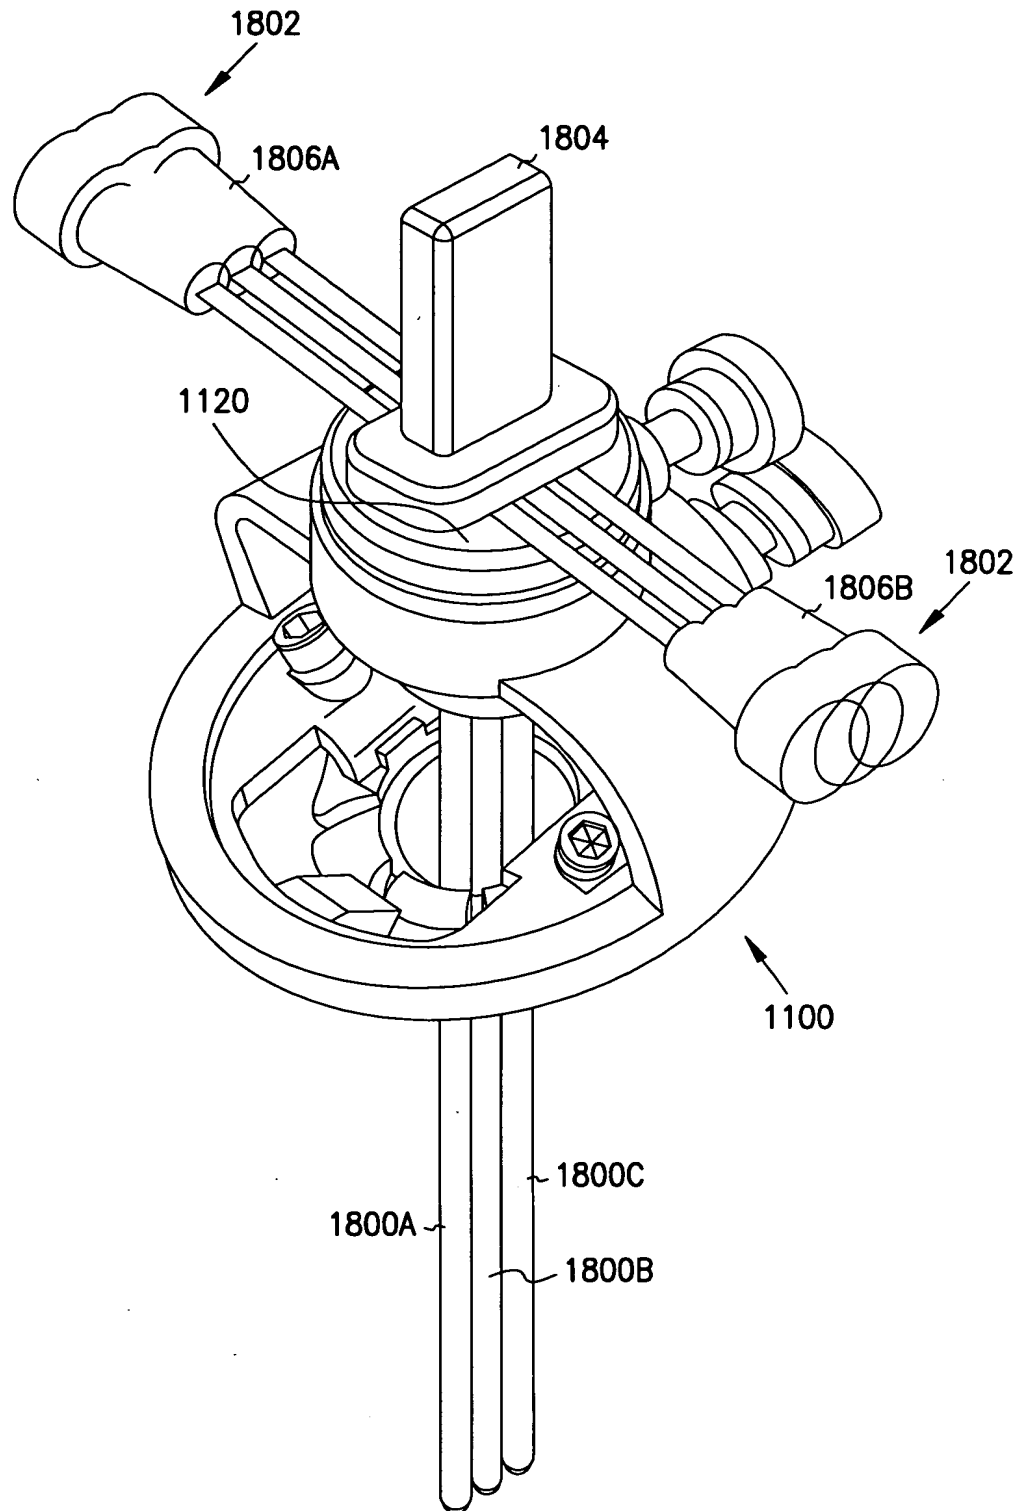


FIG. 18

09/828,451 15482350

18/36

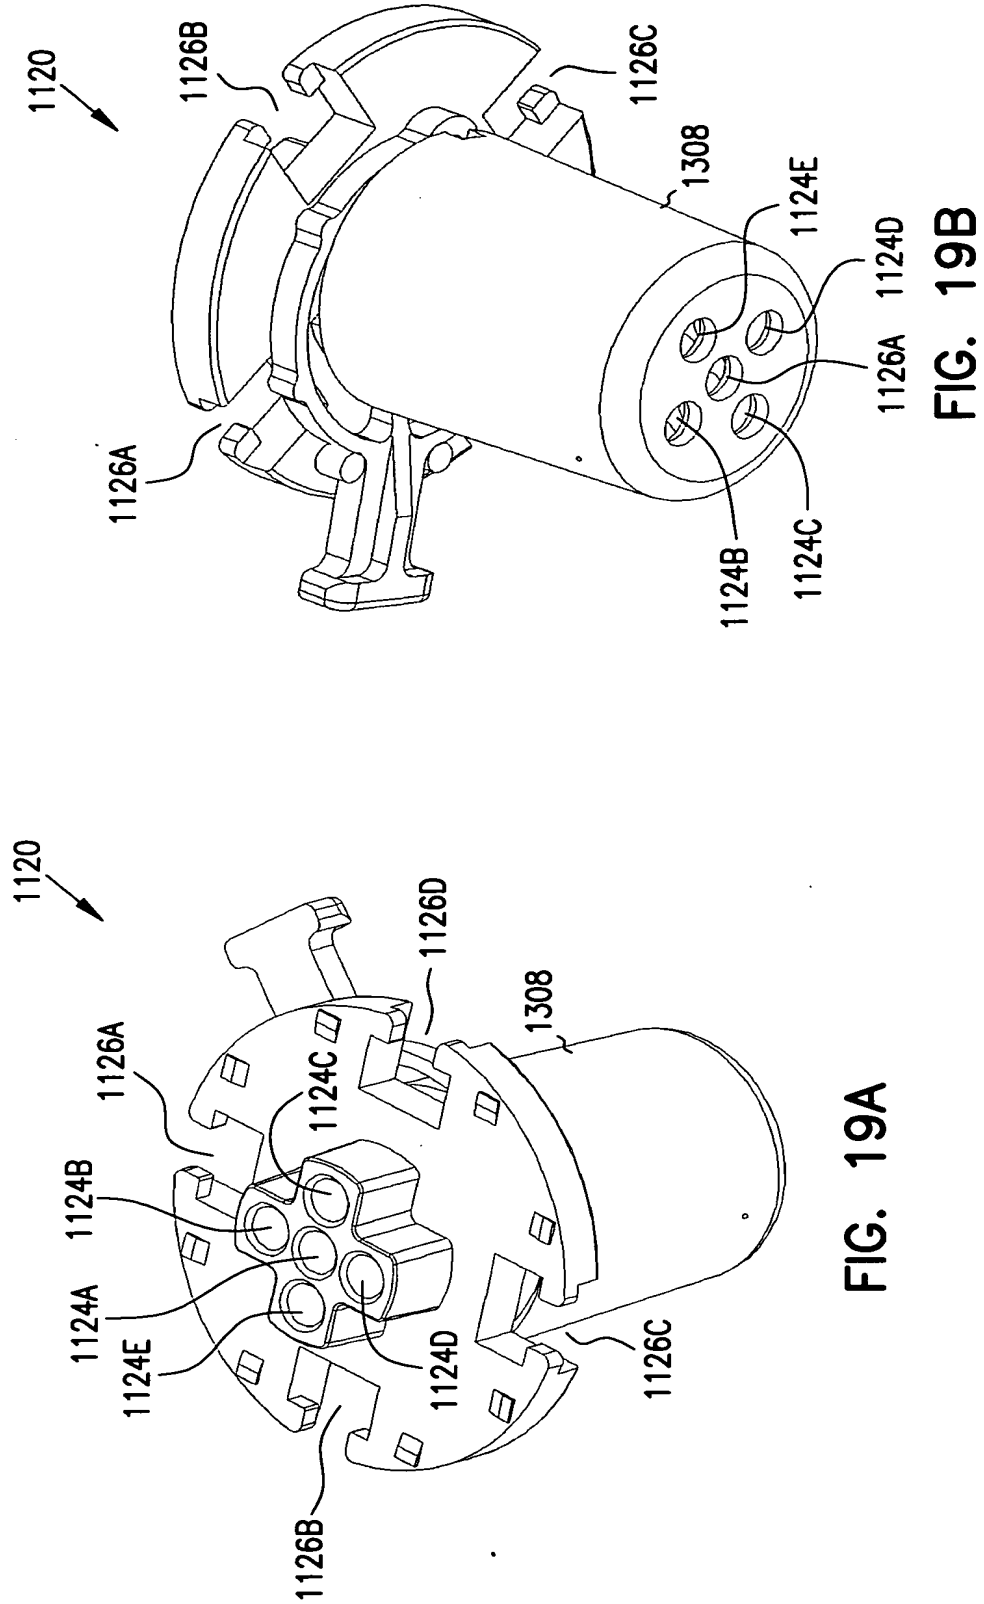


FIG. 19A

FIG. 19B

FIG. 19A

19/36

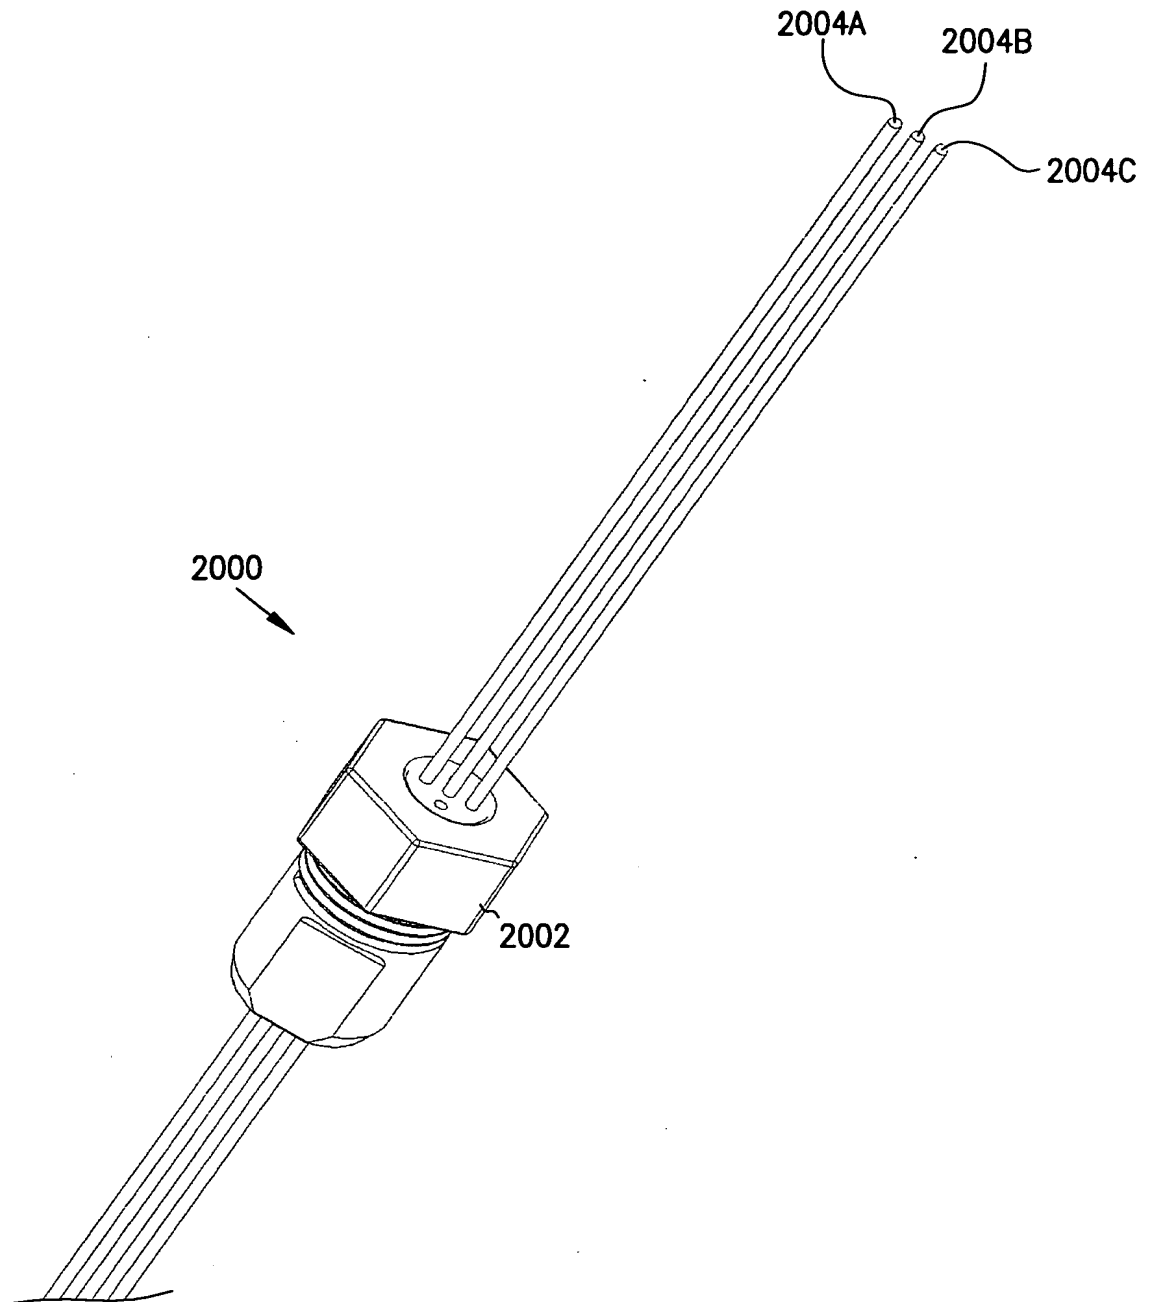


FIG. 20

09828451.082001

20/36

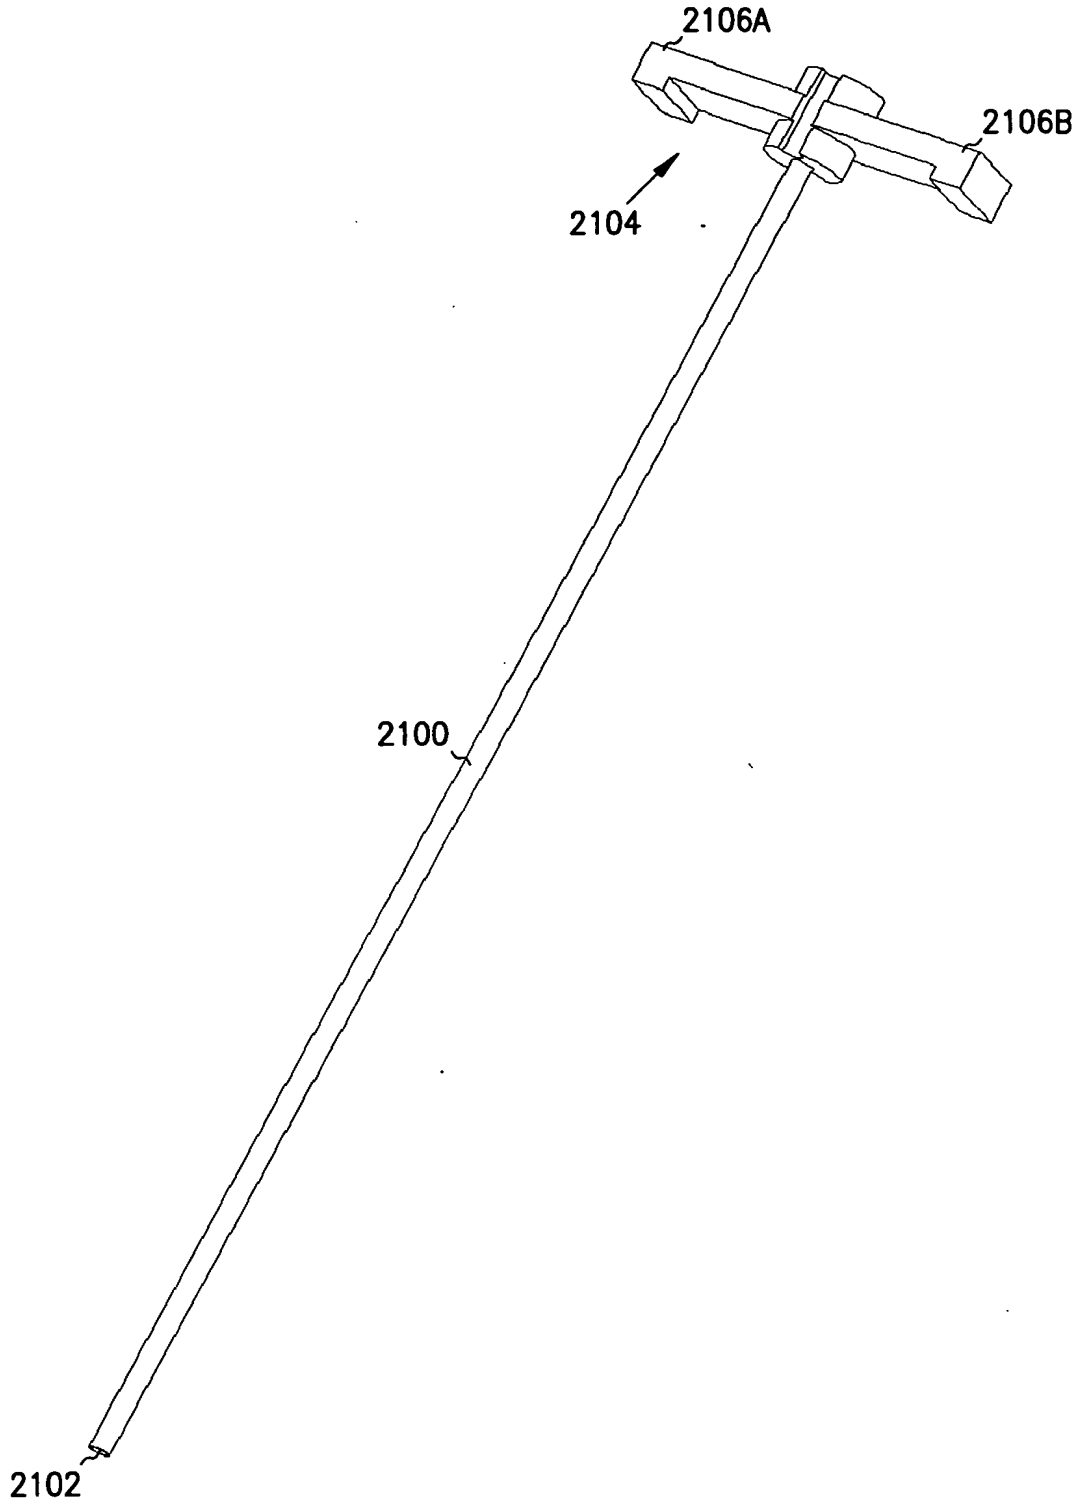


FIG. 21

09828451 082001

21/36

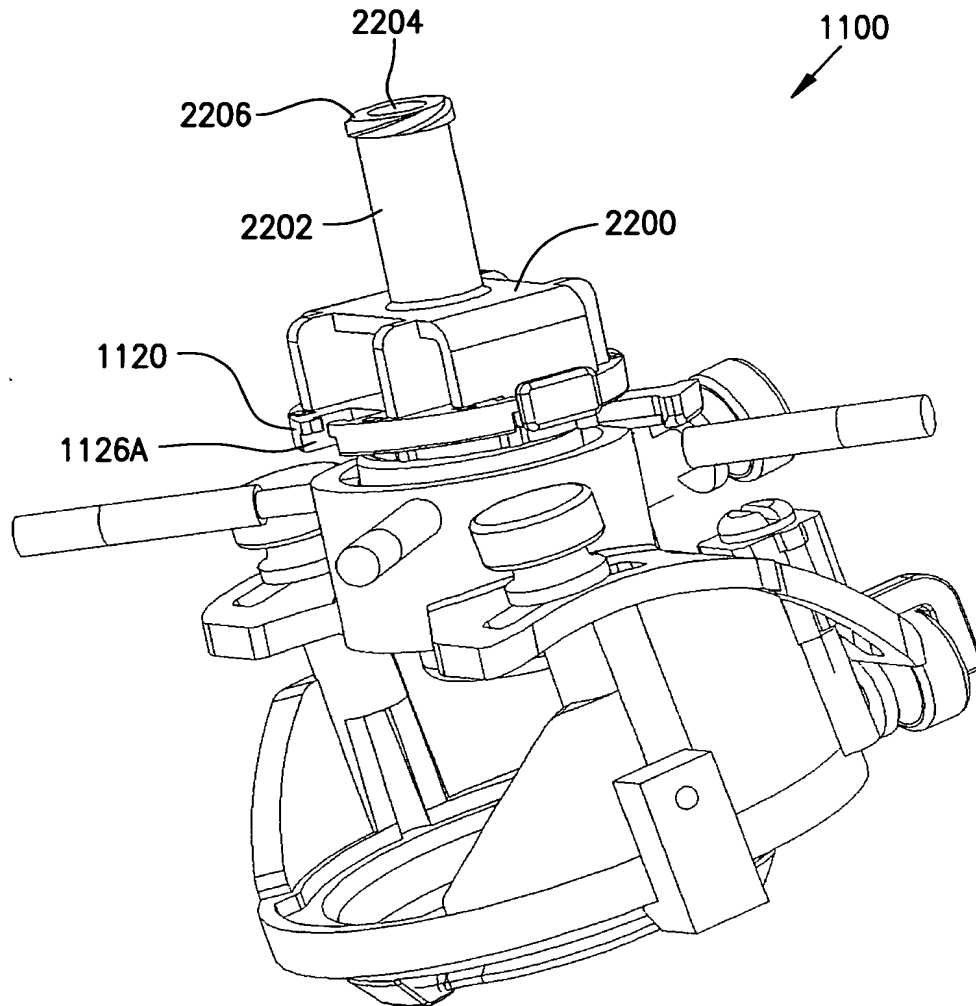


FIG. 22

09/828,451 "T 5422601

22/36

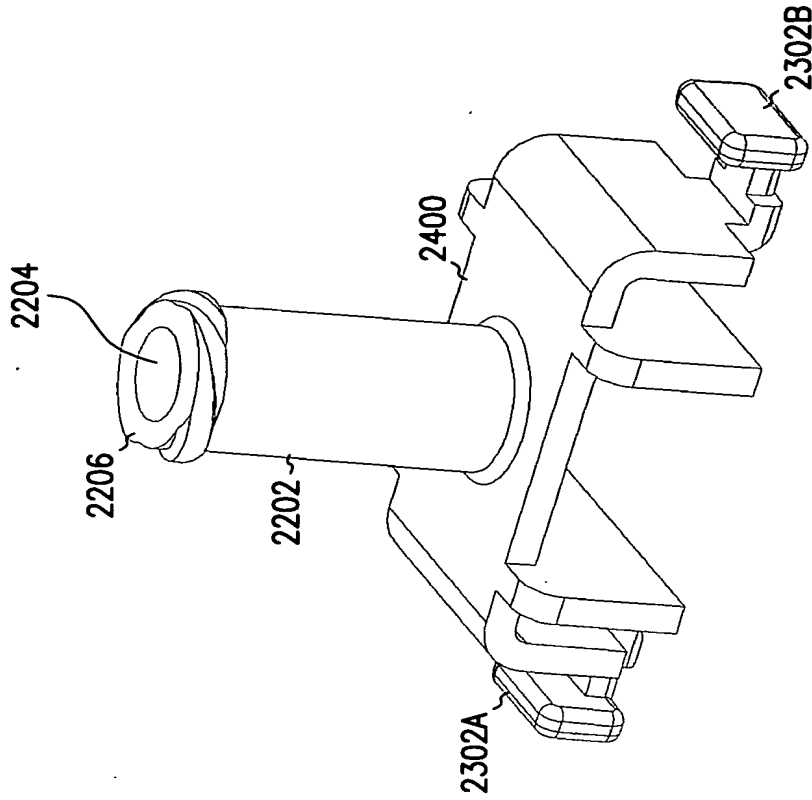


FIG. 24

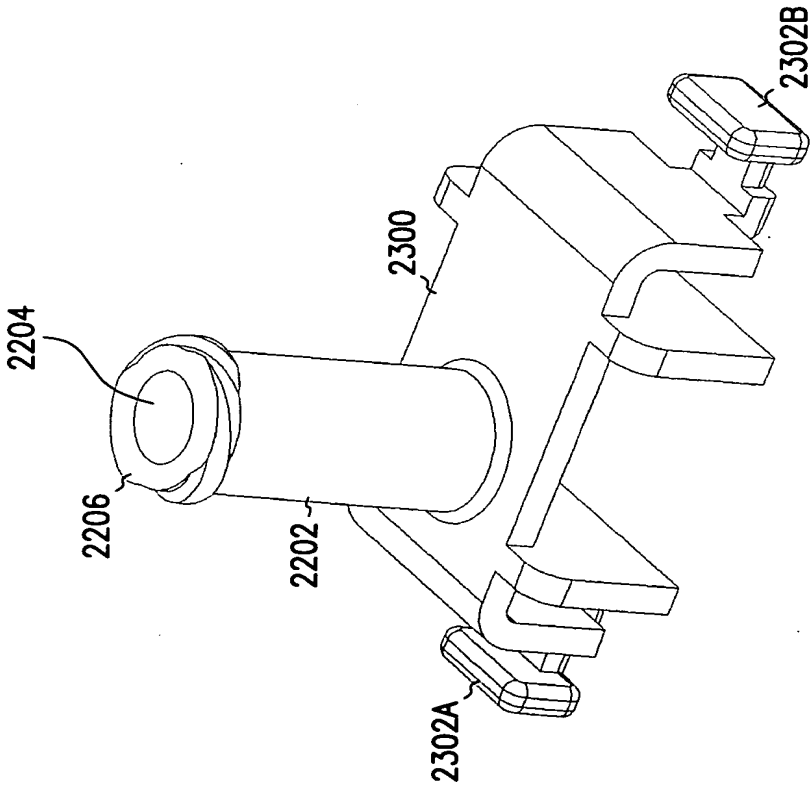


FIG. 23

TI DEEP ORGAN ACCESS DEVICE AND METHOD

23/36

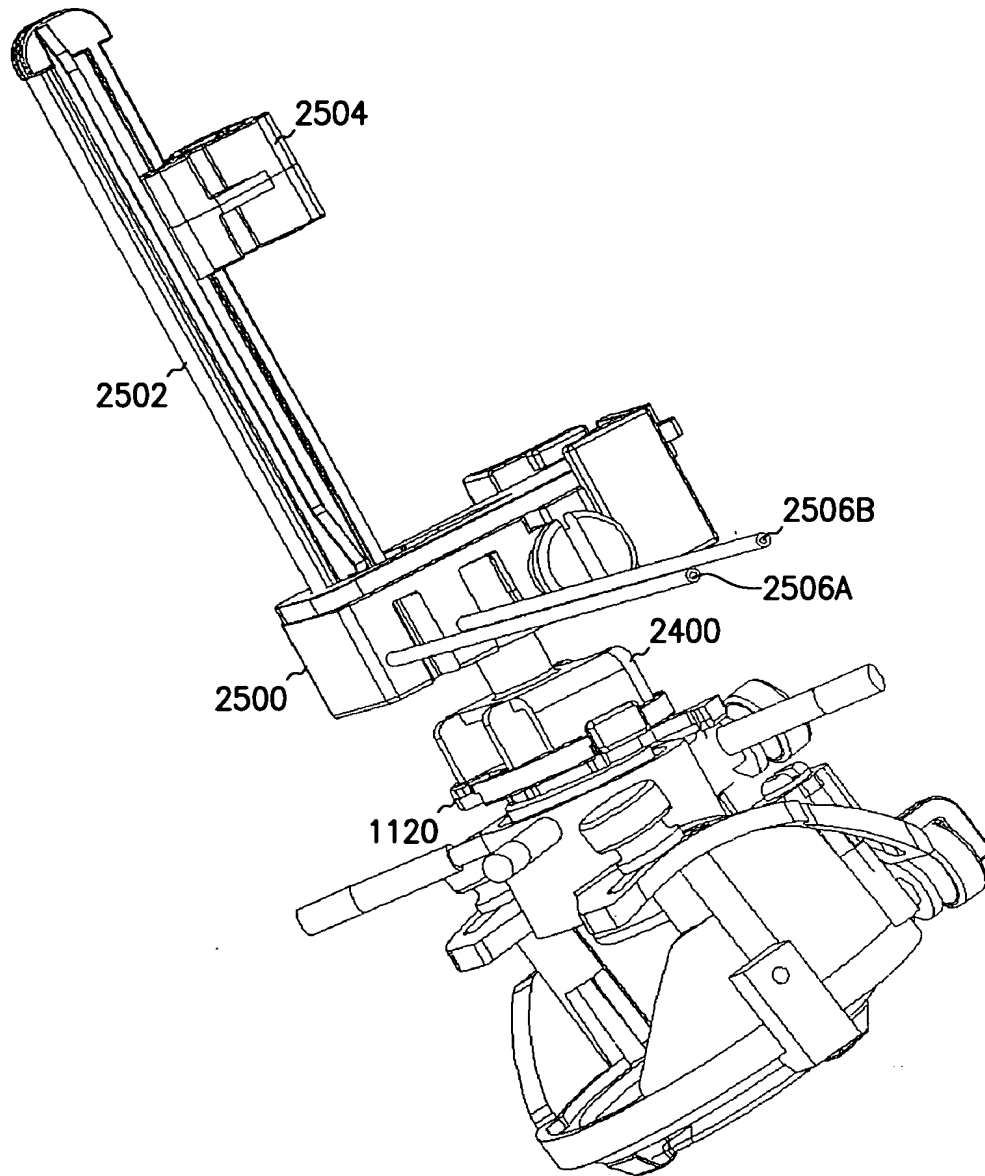


FIG. 25

09/828,451, 082001

24/36

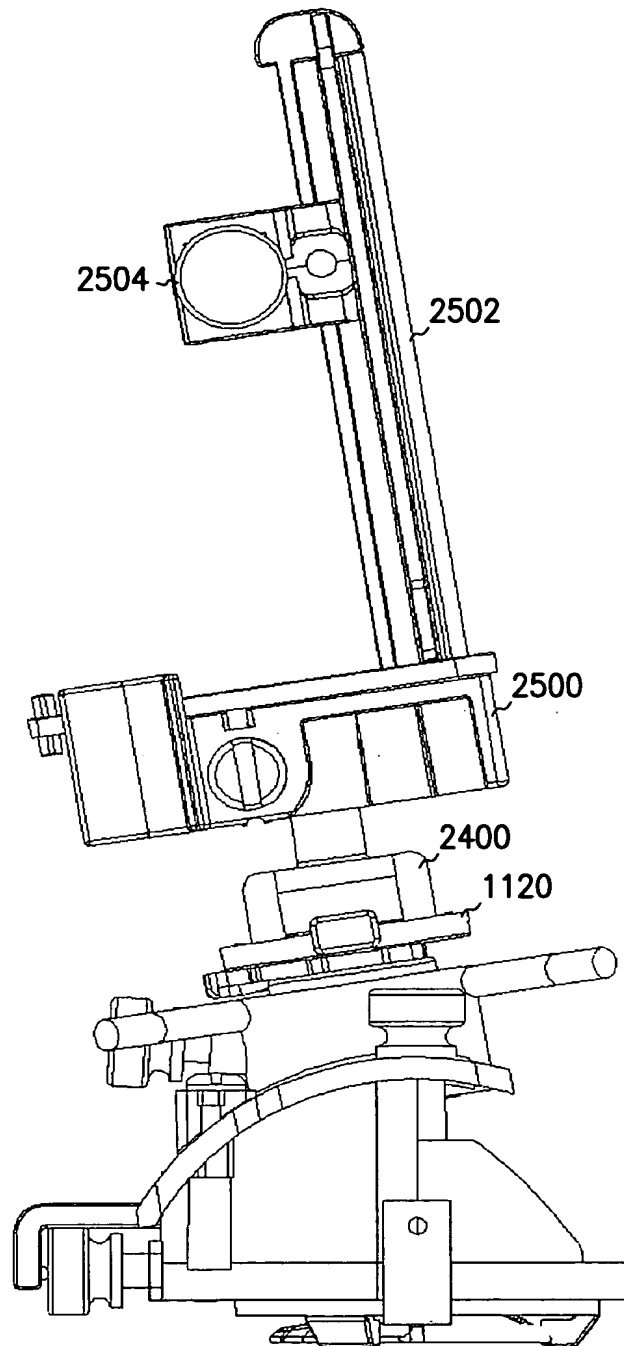


FIG. 26

09828451 00000000



25/36

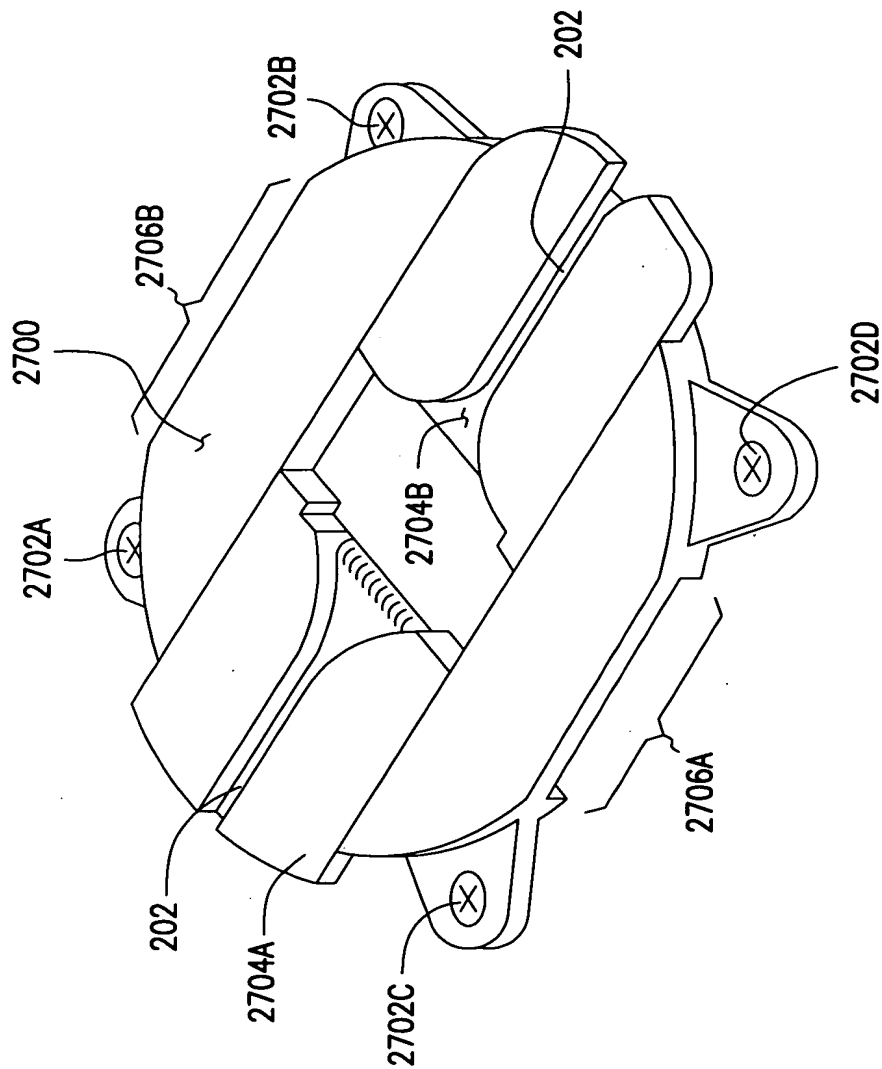


FIG. 27

TI DEEP ORGAN ACCESS DEVICE AND METHOD

26/36

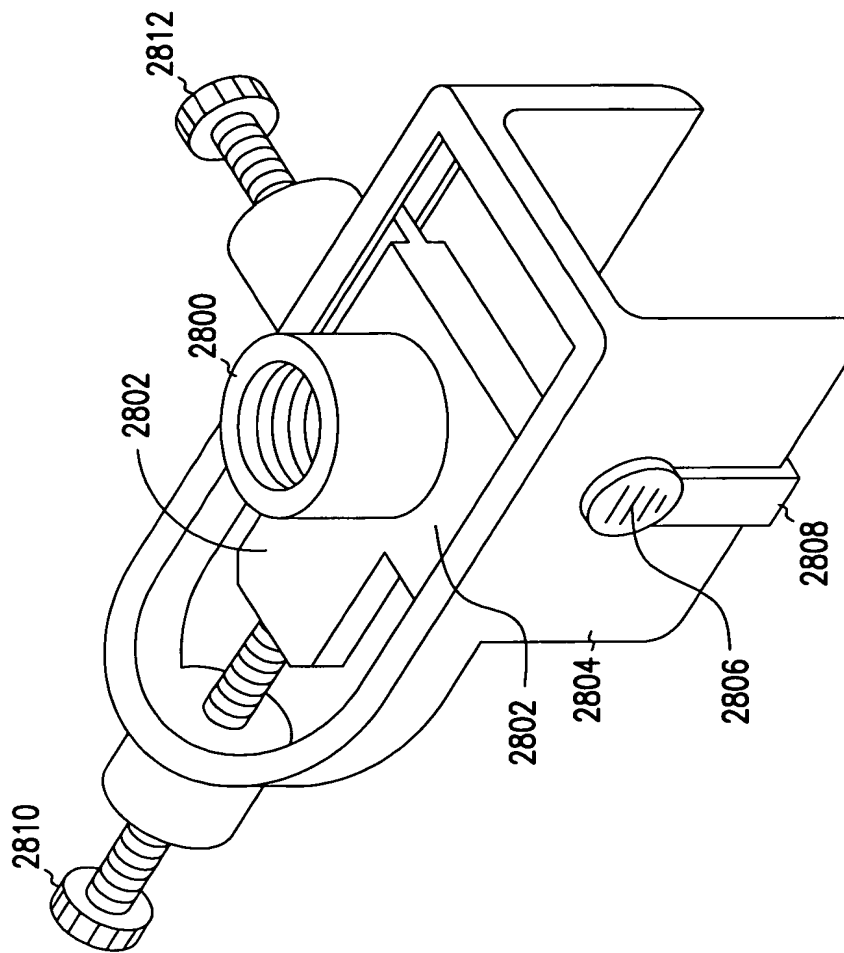


FIG. 28

FIG. 28 of 5432360

27/36

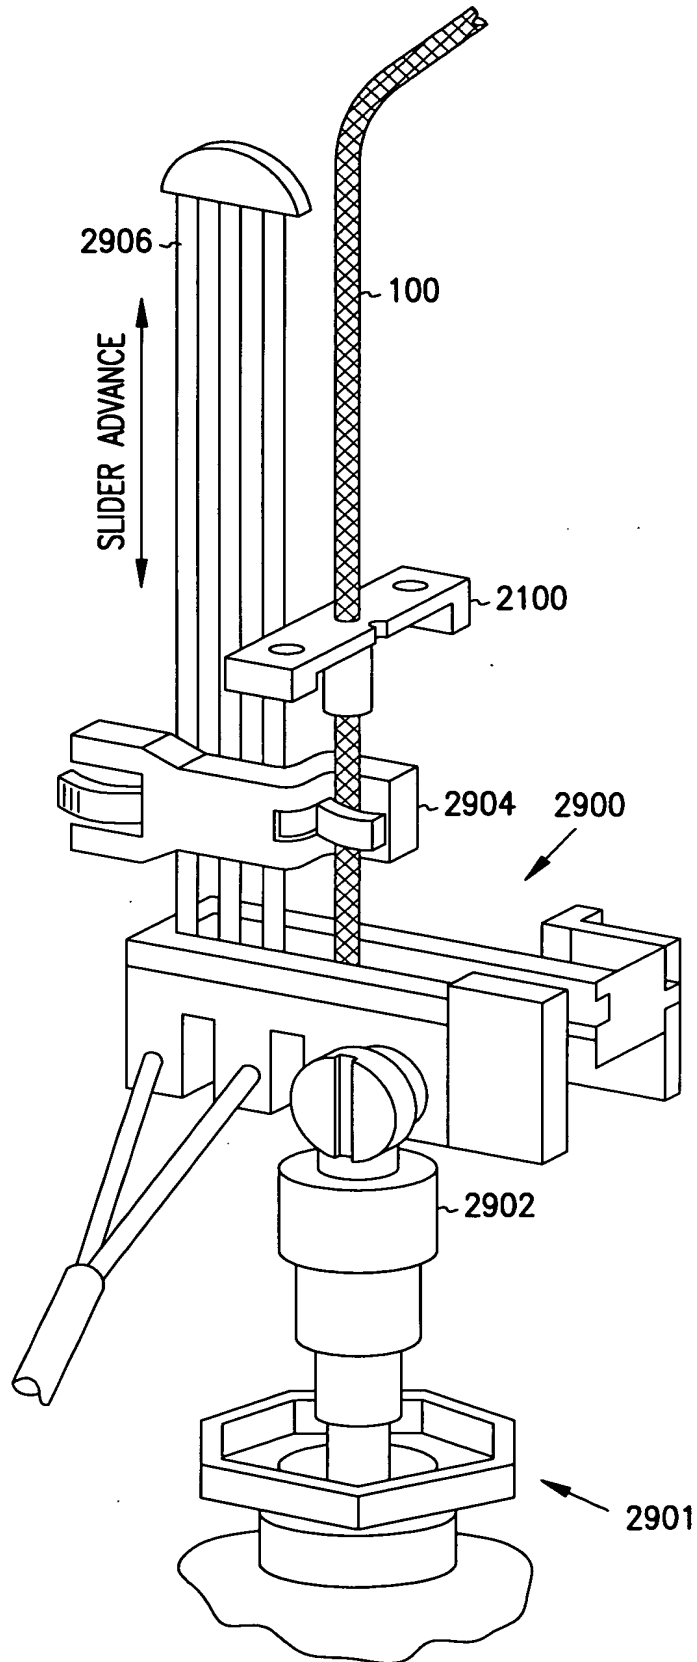


FIG. 29

09828451 15482860

28/36

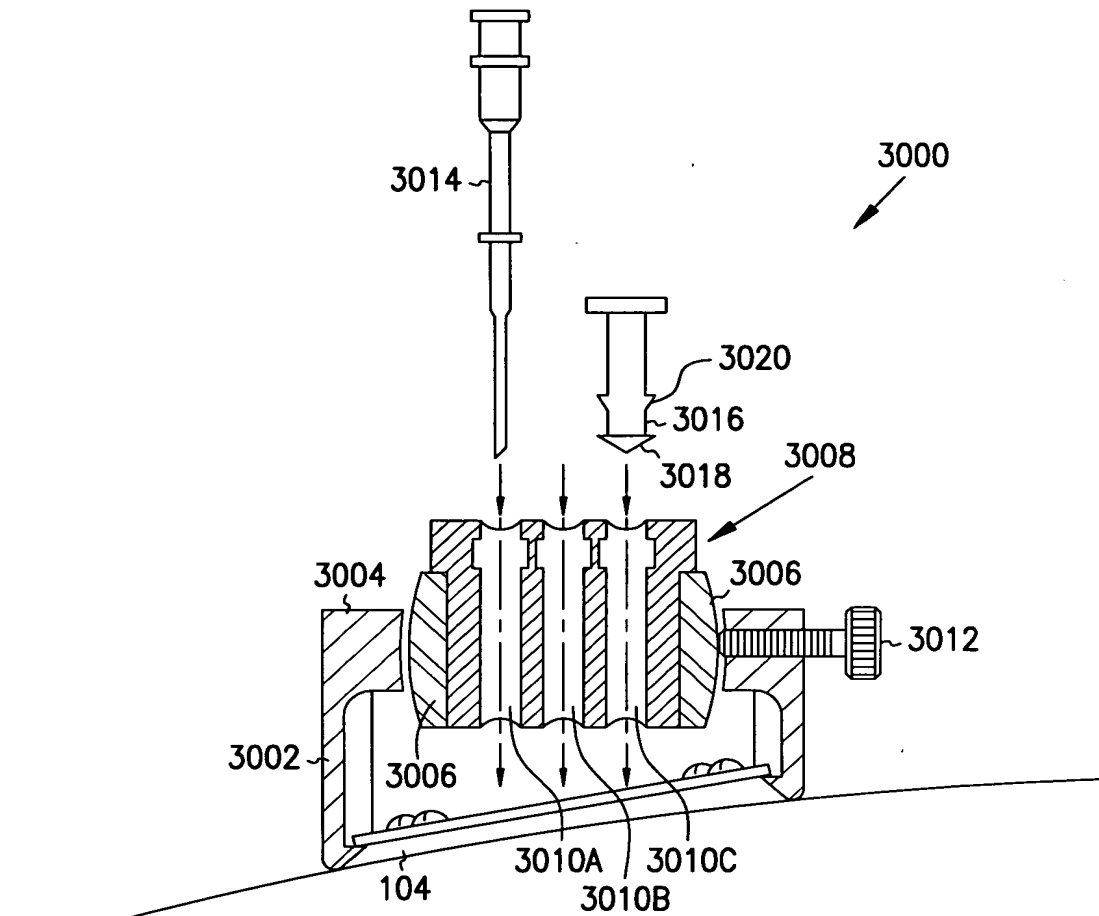


FIG. 30

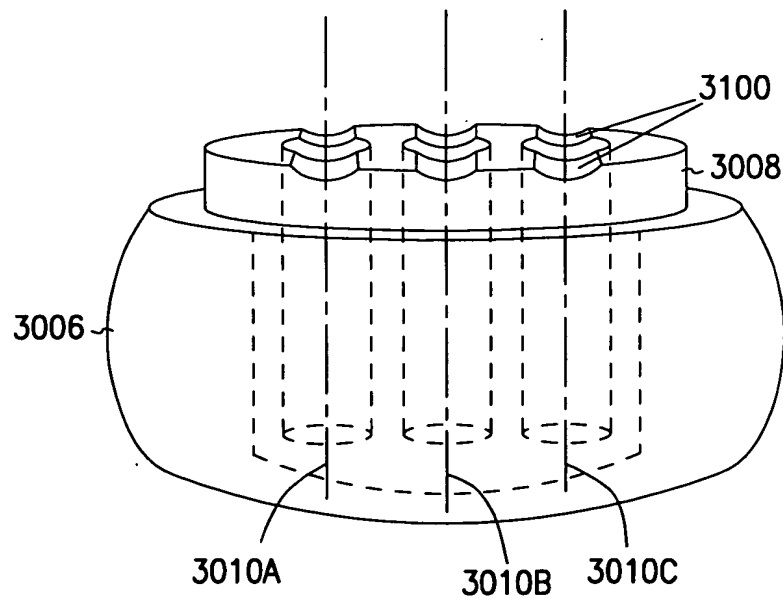


FIG. 31

29/36

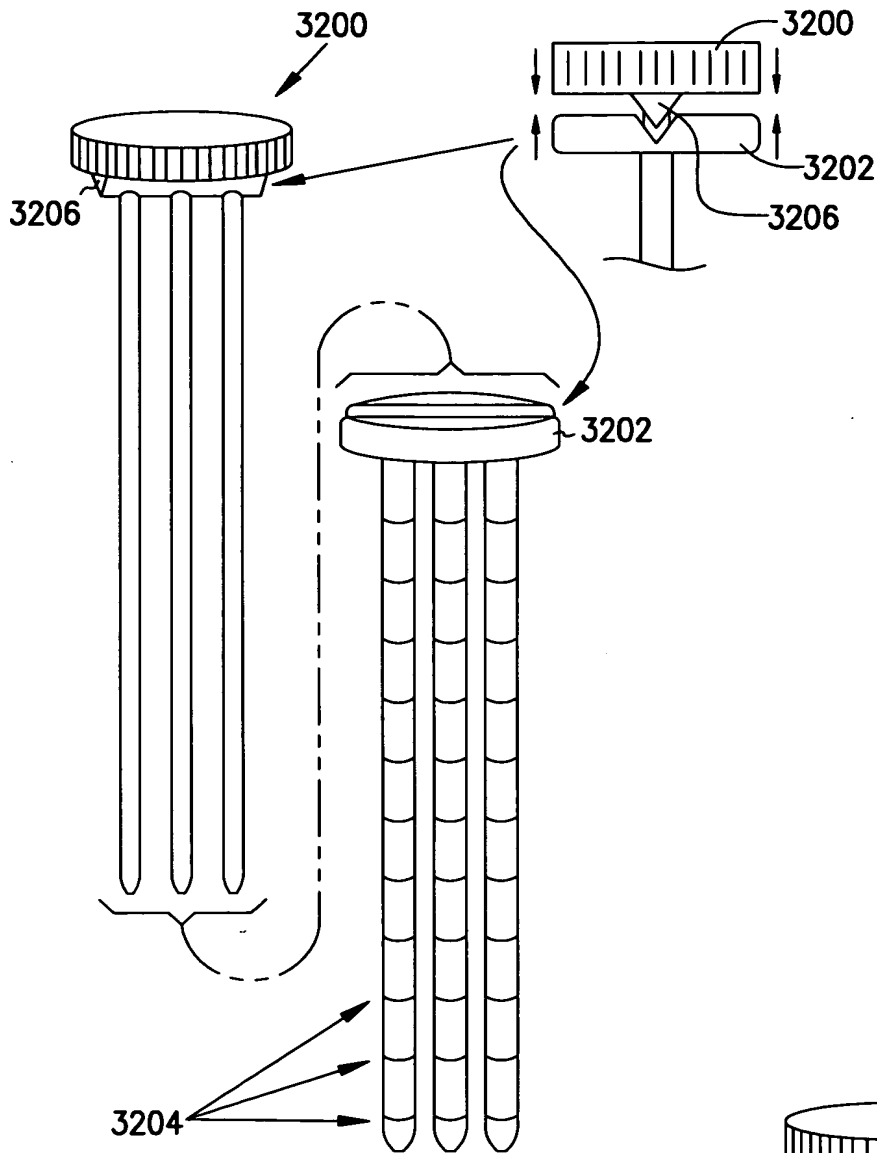


FIG. 32A

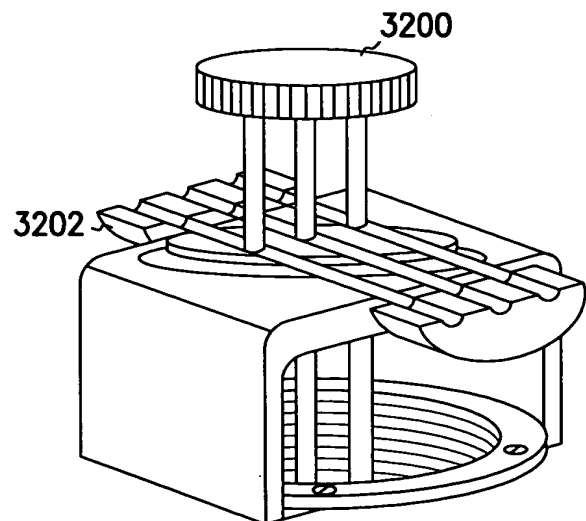


FIG. 32B

FIG. 33A

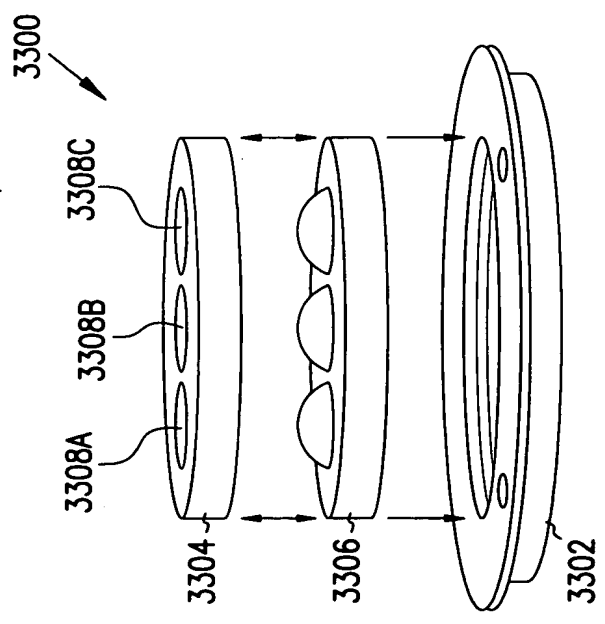


FIG. 33A

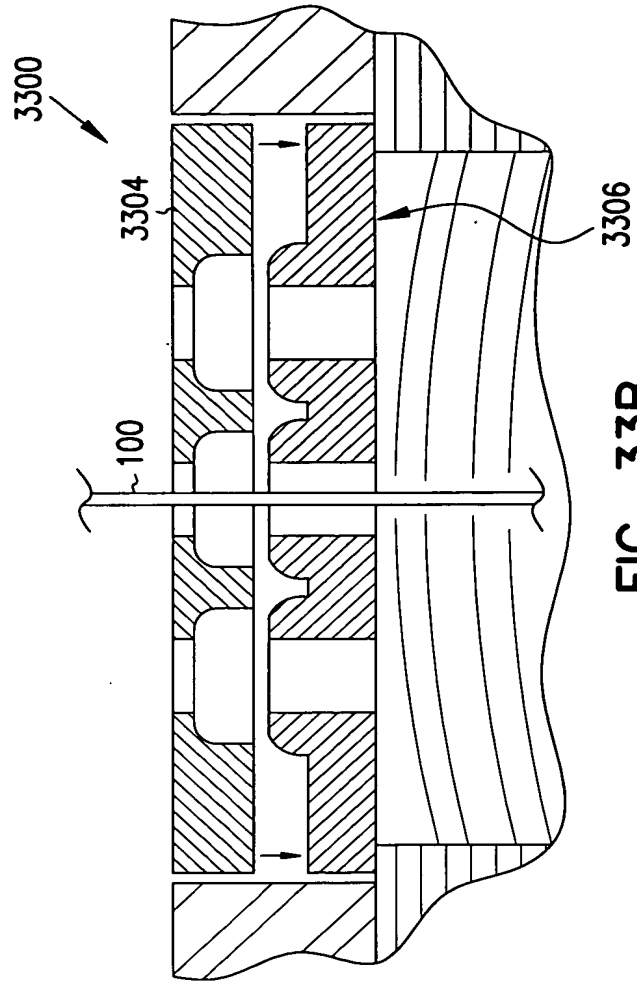


FIG. 33B

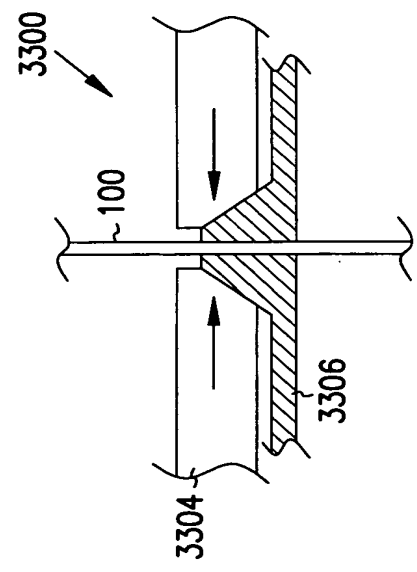


FIG. 33C

31/36

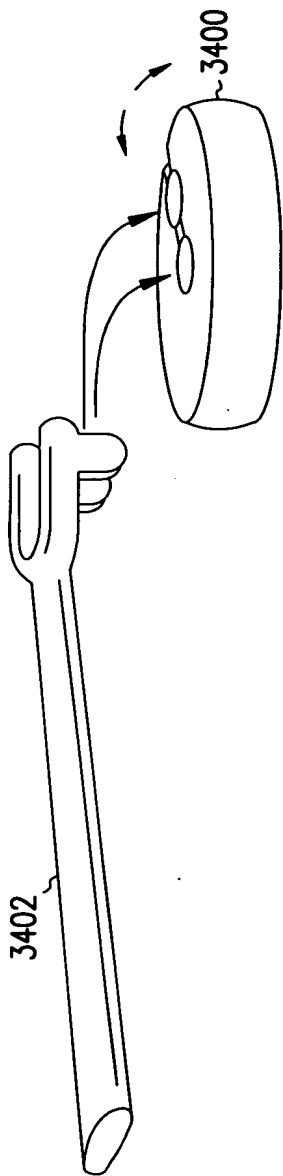


FIG. 34A

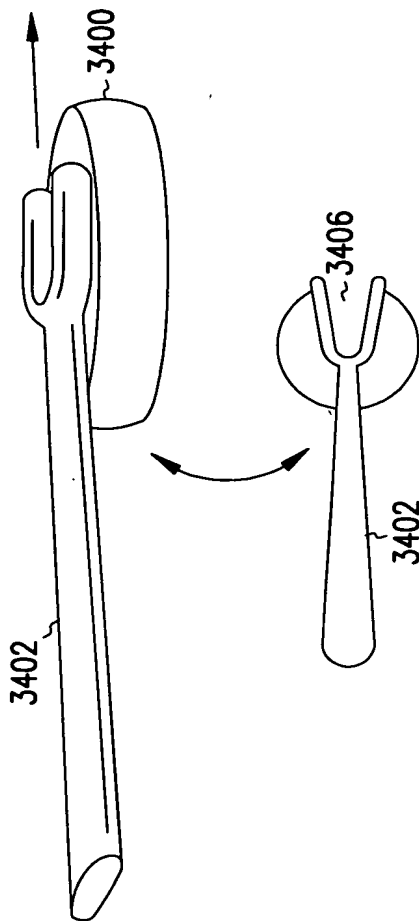


FIG. 34B

T00280 T5482860

32/36

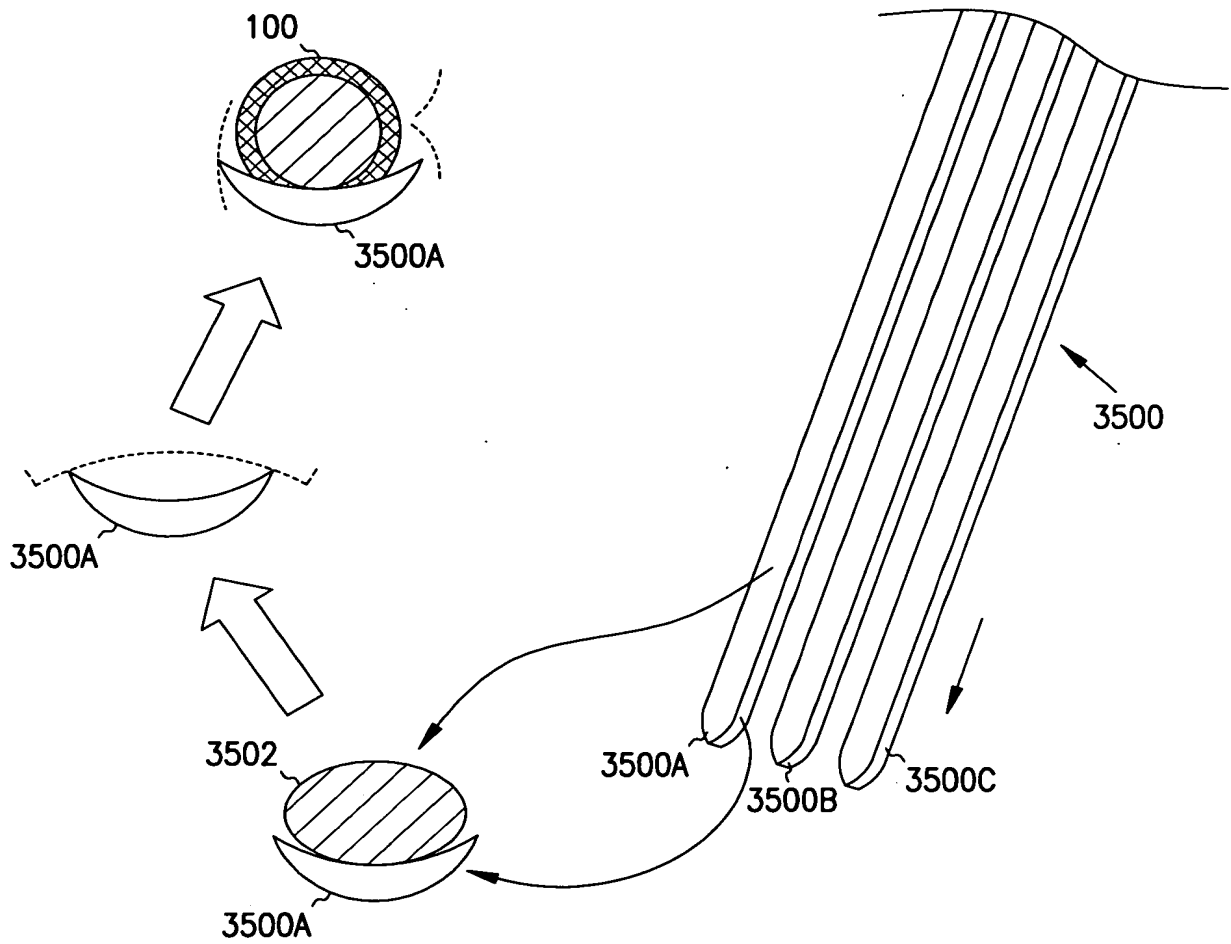


FIG. 35

09/828,451, 08/26/01



33/36

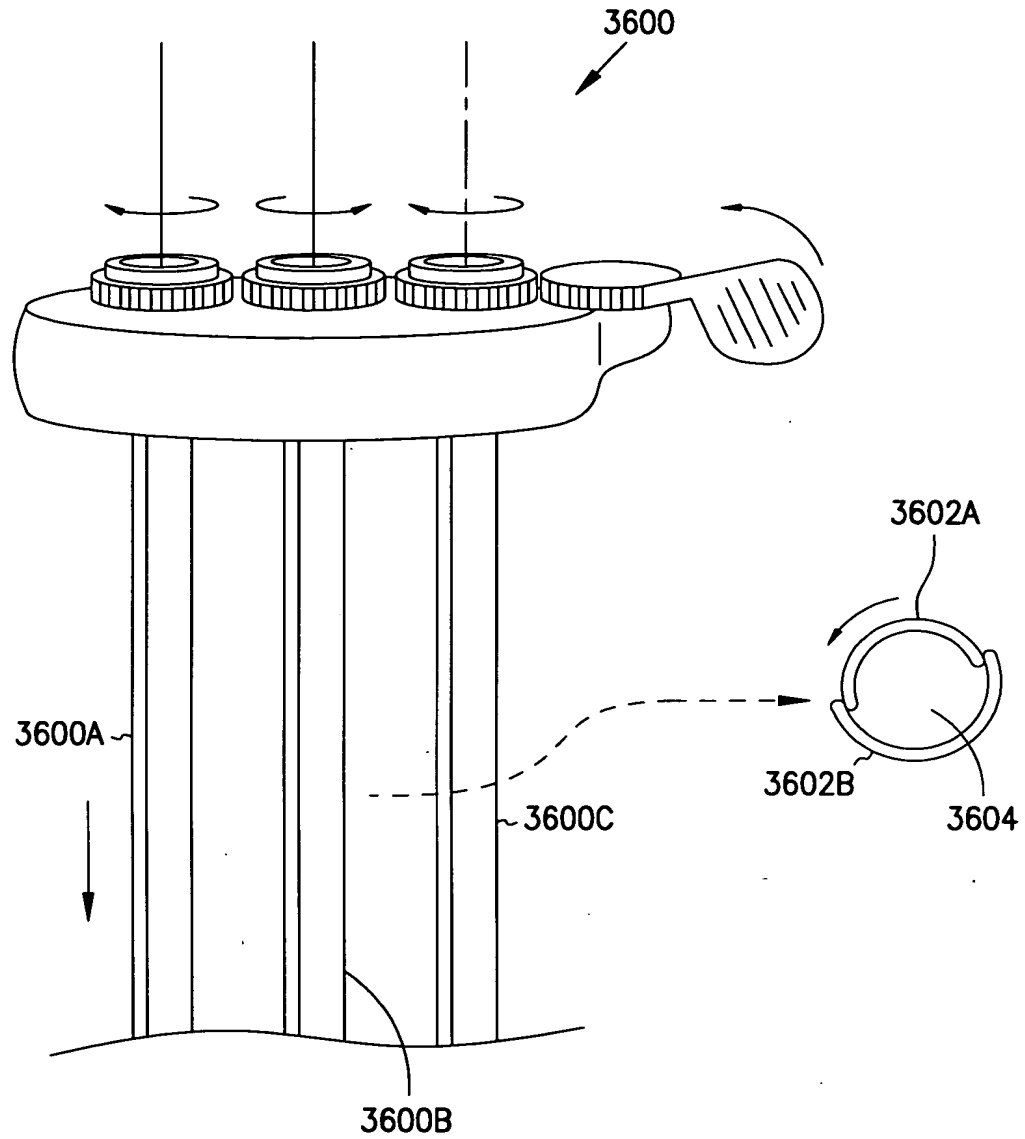


FIG. 36

34/36

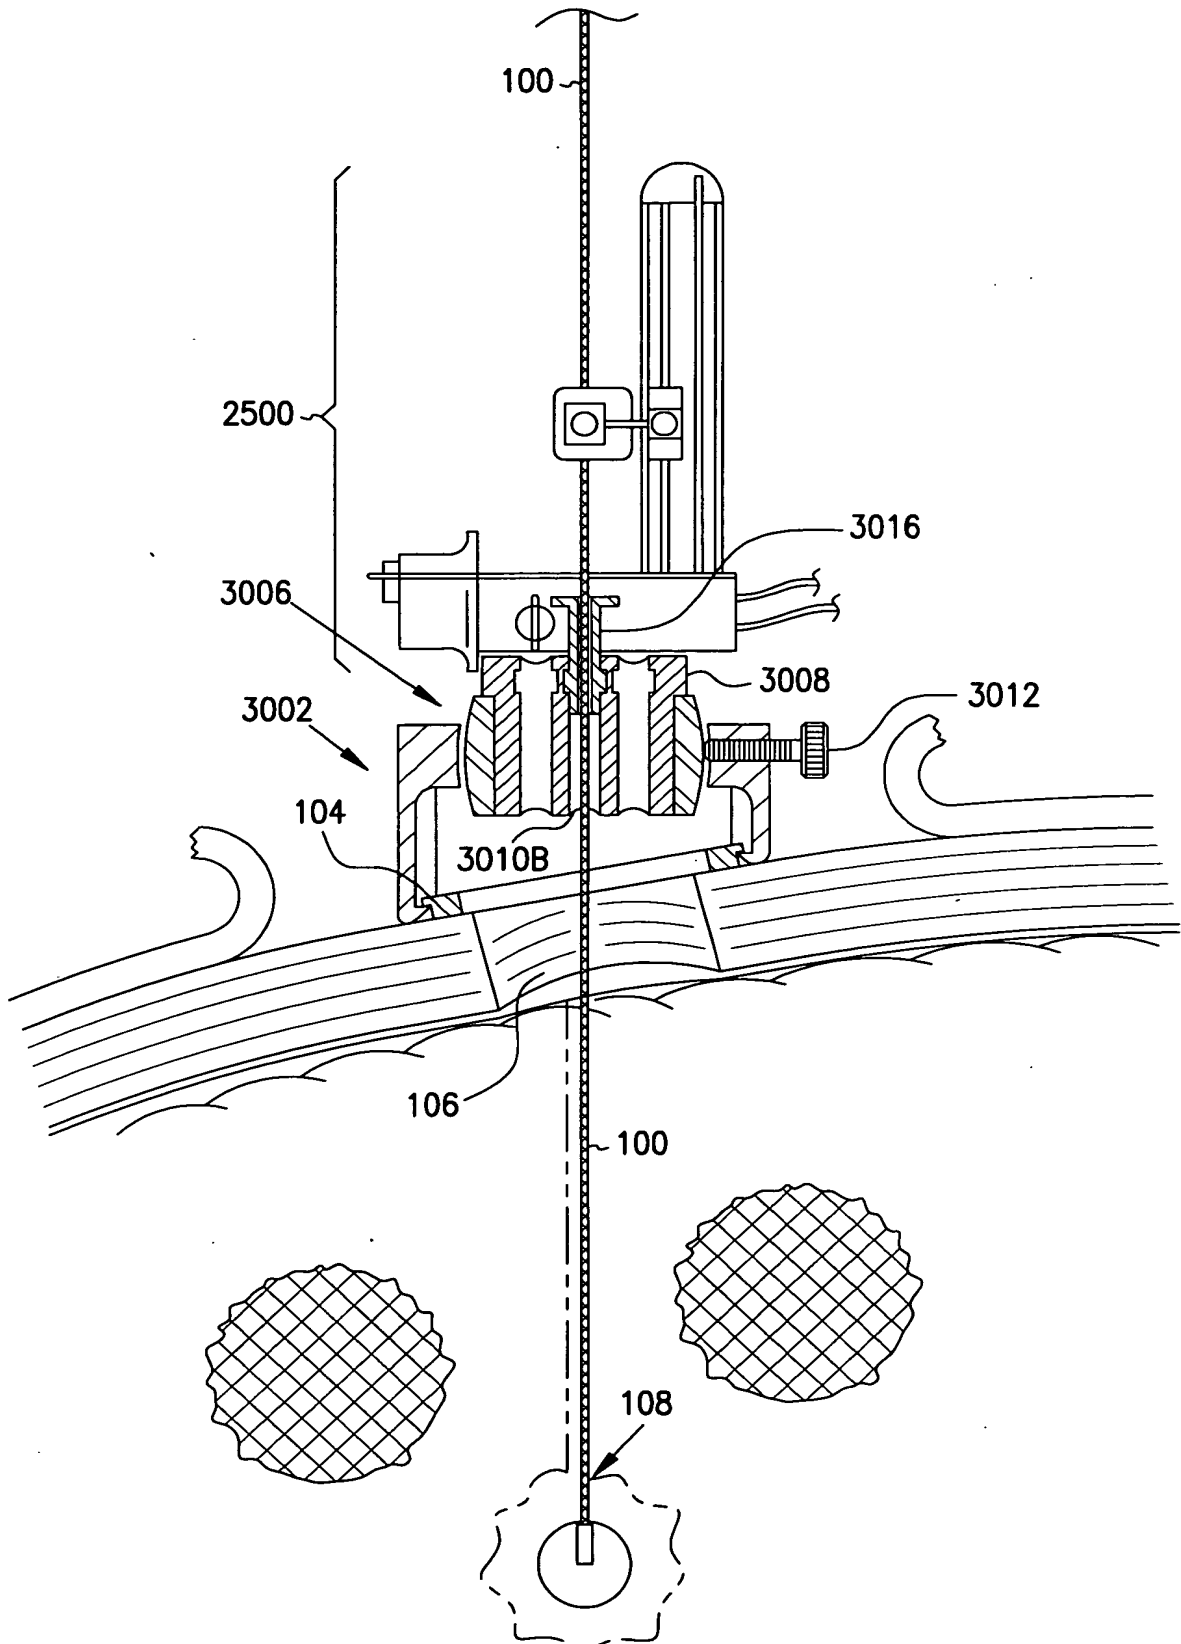


FIG. 37

35/36

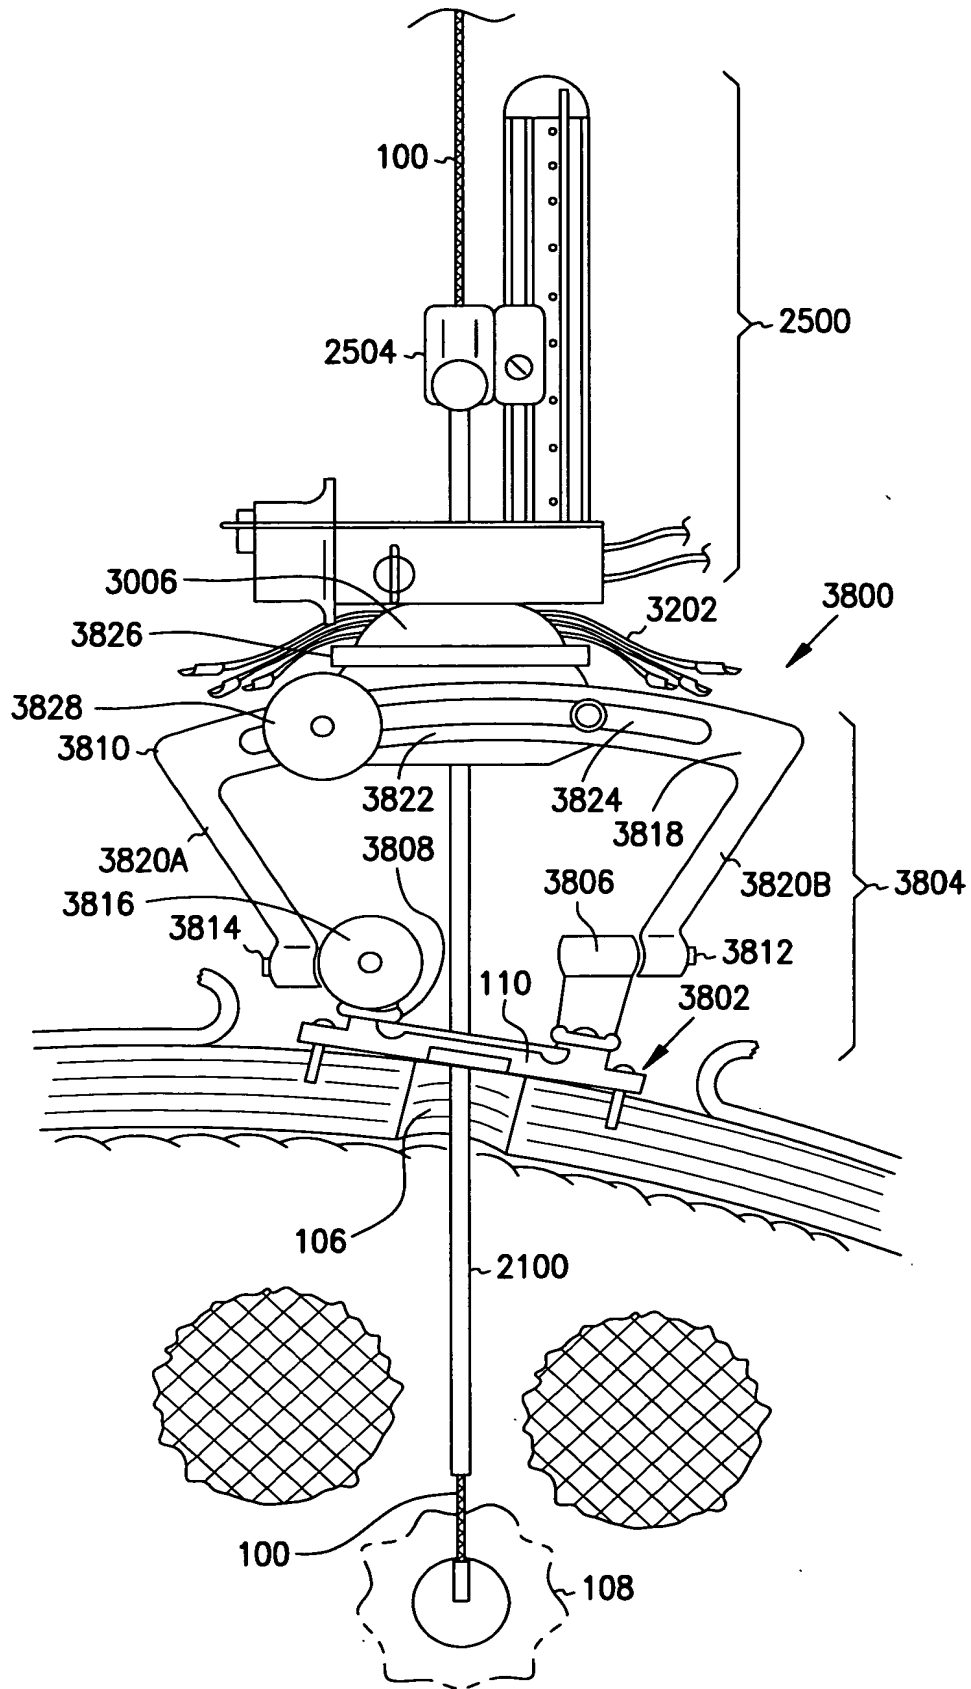


FIG. 38

09828451-08001

36/36

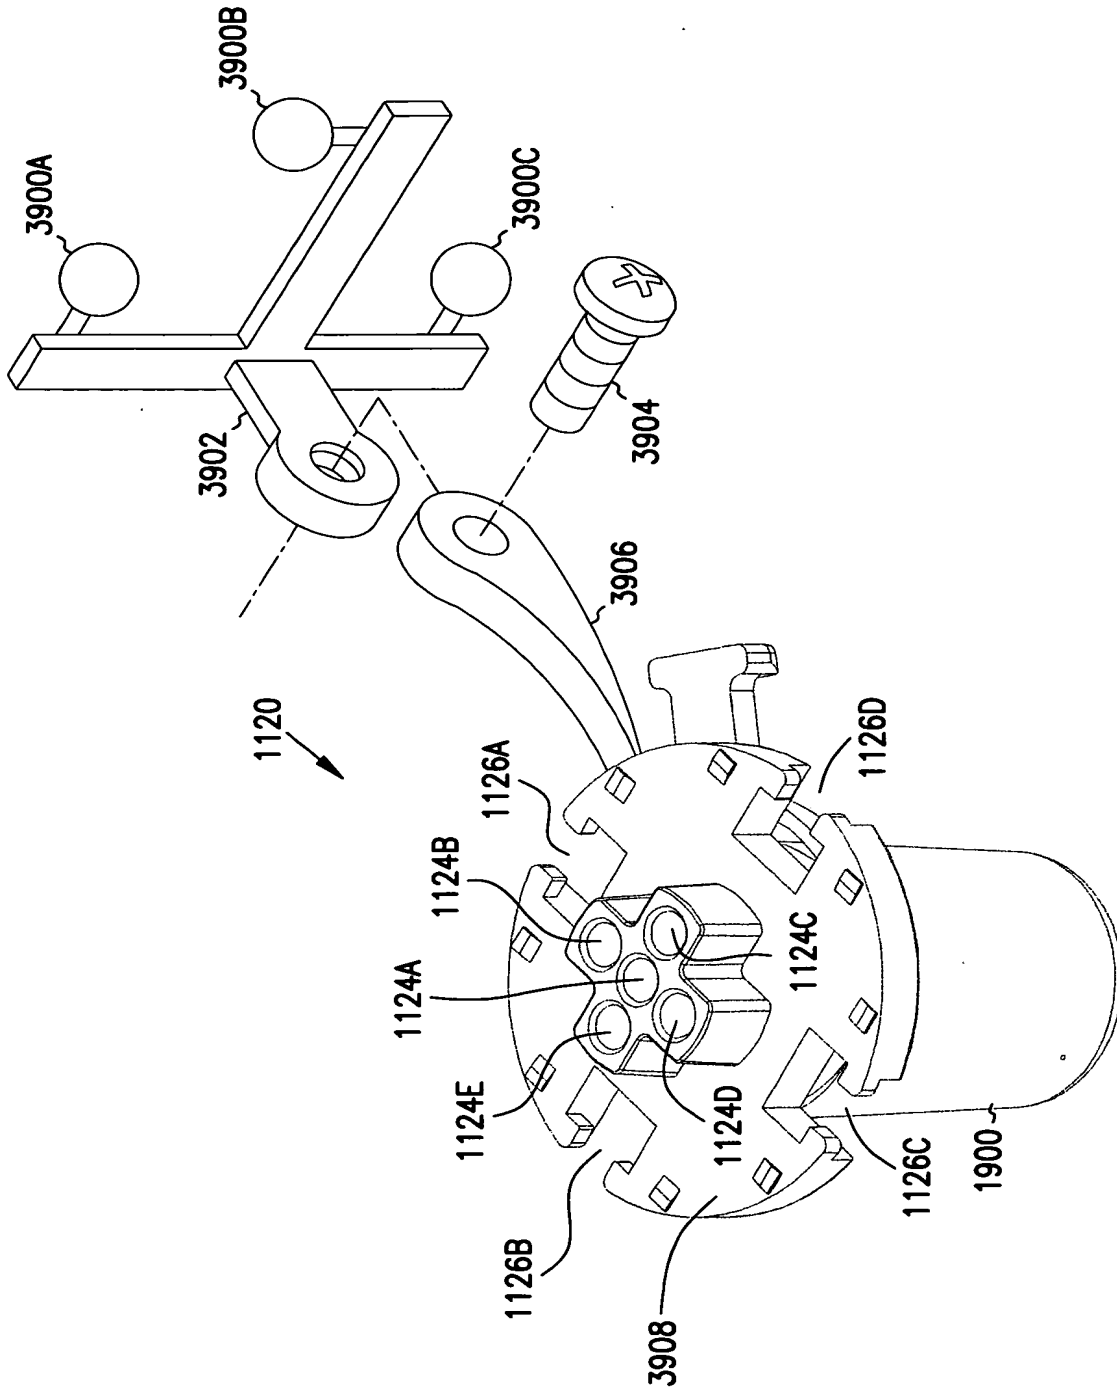


FIG. 39

T00280" T5482860